

Meta-analysis of rapid direct-to-PCR assays for the qualitative detection of SARS-CoV-2

Team

R.A. Trevor, S. Gripton, H. Chen, L. Koh, D.

Borley, P. Oladimeji, Stephen P. Kidd*, J.E.

Martin*

*joint senior authors

Contact

Daryl Borley

Date completed

03/05/2021

Abstract

Infection with severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) and the ensuing COVID-19 pandemic present significant challenges to current diagnostic and therapeutic patient care pathways including whether new *in vitro* diagnostic tests can accurately identify and rule out current SARS-CoV-2 infection.

The gold standard diagnostic test to identify a current SARS-CoV-2 infection is a central laboratory-based molecular assay using reverse transcription polymerase chain reaction (RT-PCR) with very high accuracy of detection but which typically requires 1-2 days turn-around for results. Therefore, rapid RTPCR assays and systems have been developed which can be deployed locally (near-patient or point of care (POC), provide faster results and not impact on already stressed central laboratory capacity. Rapid test results can be returned within the same clinical encounter, facilitating timely decisions that optimise the patient care pathway and support more rapid COVID-19 diagnosis, isolation and contact tracing activities¹.

Direct-to-PCR is an evolution of RT-PCR in which the patient sample is added directly to an amplification reaction without being subjected to prior nucleic acid extraction, purification, or quantification to reduce the time and monetary resources required to process samples.¹ Rapid, direct-to-PCR systems further increase the speed of testing by combining rapid PCR instruments with direct-to-PCR assays, to generate results in less than two hours. This appears to be the first meta-analysis assessing the accuracy of rapid direct-to-PCR in the detection of SARS-CoV-2. In total, 10,957 unique records were identified and screened using a search string evaluation, 420 full-text reports and/or supplemental materials were assessed for inclusion. This resulted in 14 studies reporting 20 datasets with 4593 patient samples (1391 positive) included in the analysis.

The overall agreement between the rapid direct RT-PCR and gold standard centralised laboratory RT-PCR was 97.1% with 93.60% positive percent agreement and 98.63% negative percent agreement. The Cohen's kappa statistical coefficient $k = 0.93$, indicating an almost perfect agreement and Youden Index = 0.92. These results indicate that direct-to-PCR assays can perform equivalently to the standard centralised laboratory PCR systems for the detection of SARS-CoV-2.

Objectives

To assess the efficacy of rapid direct-to-PCR assays and systems for the detection of SARS-CoV-2 in the hospital, care home and medical research population in England from November 2020 to April 2021.

Search methods

Electronic searches of the Cochrane COVID-19 Study Register (which includes daily updates from PubMed and Embase and preprints from medRxiv and bioRxiv) were undertaken on the 30th of April 2020. Please see the PRISMA flow diagram below (figure 2).

Selection criteria

Studies of subjects with either suspected SARS-CoV-2 infection, known SARS-CoV-2 infection or known absence of infection, or those who were being screened for infection were included. Commercially available and research use rapid direct-to-PCR assays (without RNA extraction and purification reporting results within two hours) were included in the study.

Data collection, extraction and analysis

Studies were screened independently, in duplicate with any disagreements resolved by discussion with a third author. Study characteristics were extracted by one author and checked by a second; extraction of study results and assessments of risk of bias and applicability were undertaken independently in duplicate.

Where studies were not publicly available, sites that undertook in-service evaluations of rapid direct-to-PCR system were contacted and asked to supply anonymised datasets. Both reviewers independently performed data extraction and verification and calculated 2x2 contingency tables of the number of true positives, false positives, false negatives and true negatives. They resolved any disagreements by discussion and by review with the third reviewer.

Main results

Twenty study cohorts were included (described in 14 study reports, including 4 unpublished reports), reporting results for 4593 samples (1391 with confirmed SARS-CoV-2). Studies were mainly from Europe and North America, and evaluated nine direct-to-PCR assays.

Conclusions

This appears to be the first meta-analysis assessing the accuracy of rapid direct-to-PCR in the detection of SARS-CoV-2. In total, 10,957 unique records were identified and screened using a search string evaluation, 420 full-text reports and/or supplemental materials were assessed for inclusion. This resulted in 14 studies reporting 20 datasets with 4593 patient samples (1391 positive) included in the analysis.

The overall agreement between the rapid direct RT-PCR and gold standard centralised laboratory RT-PCR was 97.10% with 93.60% positive percent agreement and 98.63% negative percent agreement. The Cohen's kappa statistical coefficient $k = 0.93$, indicating an almost perfect agreement and Youden Index = 0.92. These results show that direct-to-PCR assay perform equivalently to the gold standard centralised laboratory RT-PCR systems for the detection of SARS-CoV-2.

Plain language summary

What is a rapid direct-to-PCR tests for diagnosing COVID-19?

Rapid direct-to-PCR tests are rapid tests that aim to confirm or rule out the presence of SARS-CoV-2 within 2 hours without complicated processing of the sample.

How accurate is a rapid direct-to-PCR tests for diagnosing COVID-19?

We compared the accuracy of rapid direct-to-PCR tests with gold standard centralised laboratory RT-PCR for the detection of SARS-CoV-2 and found that direct-to-PCR was as accurate as standard RT-PCR assays.

Why is this question important?

People with suspected COVID-19 need to know quickly whether they are infected, so that they can self-isolate, inform close contacts and possibly receive treatment. Currently, COVID-19 infection is confirmed by a laboratory test called RT-PCR, which uses specialist equipment and often takes at least 24 hours to produce a result. If they

are accurate, faster diagnosis could allow people to take appropriate action more rapidly, with the potential to reduce the spread of COVID-19.¹

What did we aim to find out?

Our goal was to determine if commercially available and research use rapid direct-to-PCR tests are accurate enough to detect SARS-CoV-2 compared to gold standard laboratory RT-PCR.

What did we do?

We looked for studies that measured the accuracy of any commercially produced and research use rapid direct-to-PCR tests, in people tested for COVID-19 using RT-PCR. People could be tested in hospital or in the community. Studies could test people with or without symptoms.

Tests had to use minimal equipment, be performed safely without risking infection from the sample, and have results available within two hours of the sample being collected.

What we found?

We included 420 studies in the review. They investigated a total of 4593 nose or throat samples; COVID-19 was confirmed in 1391 of these samples. The studies investigated nine different direct-to-PCR tests. They took place mainly in Europe and North America.

What did we find?

Although overall results for diagnosing and ruling out COVID-19 were good (93% of infections correctly diagnosed and 99% correctly ruled out), we noted a difference in COVID-19 detection between tests, but we cannot be certain about whether results will remain the same in a real-world setting. We could not investigate differences in people with or without symptoms, nor time from symptom onset because the studies did not provide enough clinical information about their participants.

How reliable were the results of the studies?

In general, the studies included followed rigorous methods in accordance with the tests intended use to detect COVID-19 and included at least two independent results to confirm or rule out COVID-19 infection. The results from different test brands varied and few studies compared multiple rapid-PCR tests. Most of the studies did not provide sufficient information to determine whether the detection levels would vary in people with COVID-19 symptoms versus without symptoms.

What does this mean?

On average the rapid direct-to-PCR were shown to be equivalent to gold standard laboratory-based RT-PCR tests and several direct-to-PCR tests show very high accuracy. However, for most of the tests, more evidence is needed particularly in people without symptoms, on the accuracy of repeated testing, testing in non-healthcare settings such as schools (including self-testing),

Background

Infection with severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) and the ensuing COVID-19 pandemic present significant diagnostic and therapeutic challenges. These range from: understanding the value of signs and symptoms in predicting possible infection; assessing whether existing biochemical and imaging tests can identify infection or people needing critical care; and evaluating whether *in vitro* diagnostic tests can accurately identify and rule out current SARS-CoV-2 infection, and identify those with past infection, with or without immunity.¹

The standard diagnostic test to identify a SARS-CoV-2 infection is a central laboratory-based molecular assay using reverse transcription polymerase chain reaction (RT-PCR).

Direct-to-PCR is an evolution of PCR in which a sample is added directly to an amplification reaction without being subjected to prior nucleic acid extraction, purification, or quantification. It allows for maximum source quantities of RNA to be targeted, minimises opportunities for error and contamination, and may be less expensive, provide results more quickly and not require the same laboratory capacity, avoiding the need for centralised testing facilities.

Rapid direct-to-PCR systems further increase the speed of testing by combining rapid-PCR instruments with faster cycling times and data analysis with direct-to-PCR assays to generate results <2 hours.

If sufficiently accurate, rapid tests returned within the same clinical encounter can facilitate the timely decisions concerning the need for isolation and contact tracing activities¹ and to facilitate novel patient care pathways for the rapid diagnosis and treatment of COVID-19, and supporting infection prevention and control.

Description of the condition

COVID-19 is the disease caused by infection with the SARS-CoV-2 virus. The target condition for this meta-analysis is current SARS-CoV-2 infection diagnosed by a positive RT-PCR detection of the SARS-CoV-2 RNA.

Description of the test

Direct-to-PCR is an evolution of RT-PCR in which a sample is added directly to an amplification reaction without being subjected to prior nucleic acid extraction, purification, or quantification. It allows for maximum quantities of source RNA to be targeted, minimises opportunities for error and contamination, and reduces the time and monetary resources required to process samples. Rapid direct-to-PCR systems further increase the speed of testing by combining rapid-PCR instruments with faster cycling times and data analysis with direct-to-PCR assays, generating results in <2 hours.

Index test(s)

The primary consideration for the eligibility of tests for inclusion in this review is that they were aimed at the detection of SARS-CoV-2 infection in samples without being subjected to prior nucleic acid extraction, purification, or quantification and with results in <2 hours.

Clinical pathway

Patients may be tested for SARS-CoV-2 when they present with symptoms, have had known exposure to a confirmed case, or are part of a screening program, with no definite known exposure to SARS-CoV-2. The standard approach to diagnosis of SARS-CoV-2 infection is through laboratory-based testing of swab samples taken from the upper respiratory (e.g., nasopharynx, oropharynx) or lower respiratory tract (e.g., bronchoalveolar lavage or sputum) with RT-PCR.¹

Rationale

It is essential to understand the clinical accuracy of tests and clinical features to identify the best way they can be used in different settings to develop effective diagnostic and management pathways for SARS-CoV-2 infection and disease. Estimates of accuracy from these reviews will help inform diagnosis, screening, isolation, and patient-management decisions.¹

Objectives

To assess the efficacy of rapid direct-to-PCR systems for the qualitative diagnosis of SARS-CoV-2 in the hospital, care home and medical research population in England from November 2020 to April 2021.

Methods

Criteria for considering studies for this review

Methods

The review was conducted following the Cochrane Rapid Review process and workflow (v.4) and we have referenced and followed the approach of the 2021 Cochrane Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection review¹. We conducted the preliminary literature search for existing or ongoing systematic reviews using the Cochrane Library and estimated review feasibility. The protocol was drafted, and a team of systematic review authors screened the titles and abstracts of all records retrieved from the literature searches following the search string optimisation described in the appendix. Two review authors independently screened studies and a third, senior review author resolved any disagreements. We tagged all records selected and obtained the full texts for all studies flagged as potentially eligible. Two review authors independently screened the full texts, and we resolved any disagreements on study inclusion through discussion with a third review author.

Assessment of Risk of Bias

The authors assessed and discussed the risk of bias and applicability concerns using the RoB 2.0 algorithm tailored to this review², and concluded that the categorization 'some concerns' was appropriate (Figure 1 below).

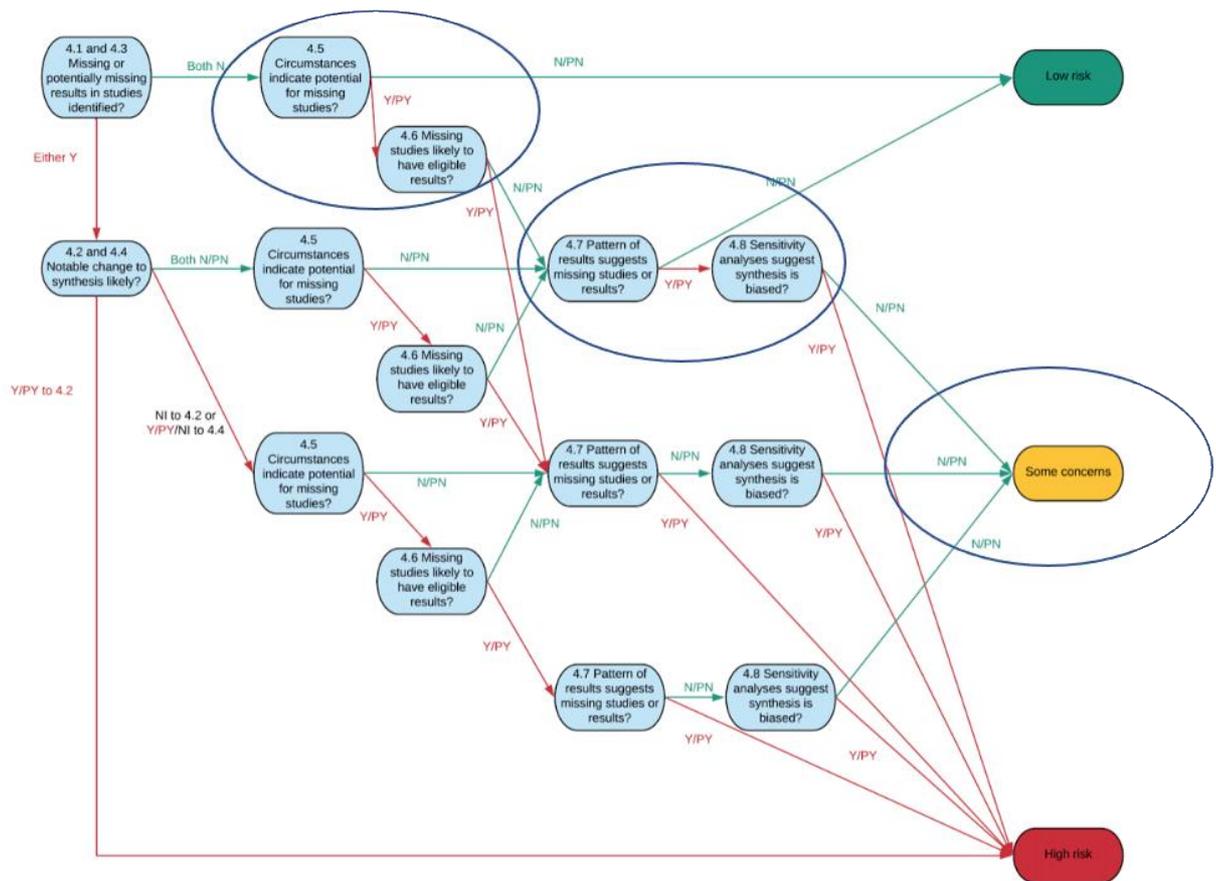


Figure 1. A tool for assessing Risk Of Bias due to Missing Evidence in a synthesis (ROB-ME)

Statistical analysis and data synthesis

We analysed rapid direct-to-PCR assays and computed estimates by summing the counts of TP, FP, FN and TN across 2x2 tables and verifying the supplemental information in publications or source data for the unpublished studies. We made comparisons between analyses using the rapid direct-to-PCR assay and standard centralized lab assay. Any discrepant results were adjudicated using a 3rd reference assay.

Assessment of reporting bias

We made no formal assessment of reporting bias but have indicated where we were aware that study results were available but unpublished.

Duration

The Minimum study duration was 1 month, and the target population encompassed symptomatic and asymptomatic residents and staff in care homes, patients in hospitals, healthcare workers and medical researchers.

Intervention

Paired nasopharyngeal, oropharyngeal or nasal patient swabs were collected. One swab from each pair was analysed using the rapid direct-to-PCR system and the other swab was tested using the gold standard centralised

laboratory PCR system. If the results were discordant, a third reference PCR system was utilised provide the definitive diagnosis.

Direct to PCR systems assessed

VitaPCR™ NAAT

SureFast® SARS-CoV-2 PLUS Test

DiaSorin Molecular Simplexa COVID-19 Direct EUA

exsig COVID-19 Direct

Hyris Kit

Simplexa

Comparator PCR systems

The New York SARS-CoV-2 Real-time Reverse Transcriptase (RT)-PCR Diagnostic EUA Panel (Modified 96 CDC assay)

Abbott ID NOW

Hologic Panther Fusion® SARS-CoV-2 EUA Hologic Panther

GenMark ePlex SARS-CoV-2 EUA panel

Cepheid

Alinity (Abbott)

M2000 (Abbott)

Roche Cobass

Genesig COVID-19

Search methods for identification of studies

Electronic databases:

Pubmed and Cochrane COVID-19 study registry from December 1st 2019 to May 2nd 2021

Other searches

Public Health England Technical Validation Group

Manufacturer websites

Unpublished NHS validation studies

Screening

Three reviewers screened all titles and abstracts for eligibility and no non-English titles were reviewed.

Data collection and analysis

Software

Excel and Sharepoint

Data extraction

Conducted with a pilot-tested form by two reviewer and verified by a third using excel to record the following:

Sample number

Exsig assay result

Exsig assay CT value

Exsig assay IC value

Comparator assay result

Comparator assay CT value

Comparator IC

Outcomes assessed: CT values to determine SARS-CoV-2

Numerical data for outcomes of interest: CT values

Contacting study authors

Authors were contacted if contingency table or source data was unavailable from the publication.

Data management

Excel and Sharepoint

Data synthesis

Published contingency tables were verified from results in the supplemental information and used to calculate overall (OPA), positive (PPA) and negative (NPA) percent agreement for published records. Source data was extracted and verified by two reviewers for unpublished studies to calculate contingency table and then calculate OPA, PPA and NPA as above.

Model

Fixed-effect meta-analysis

Analysis

Overall, percent positive and percent negative agreement, Cohen kappa (statistical coefficient to measure the agreement) and the Youden Index were calculated.

Results

Description of studies

Results of the search

10,957 unique records (published or preprints) were screened for inclusion. 420 records were selected for further assessment by review of the abstract and / or full-text reports and 103 studies for review of full-text reports and / or supplemental materials. Fourteen reports were selected for requiring assessment for inclusion in this review. See Figure 2 for the PRISMA flow diagram of search and eligibility results.

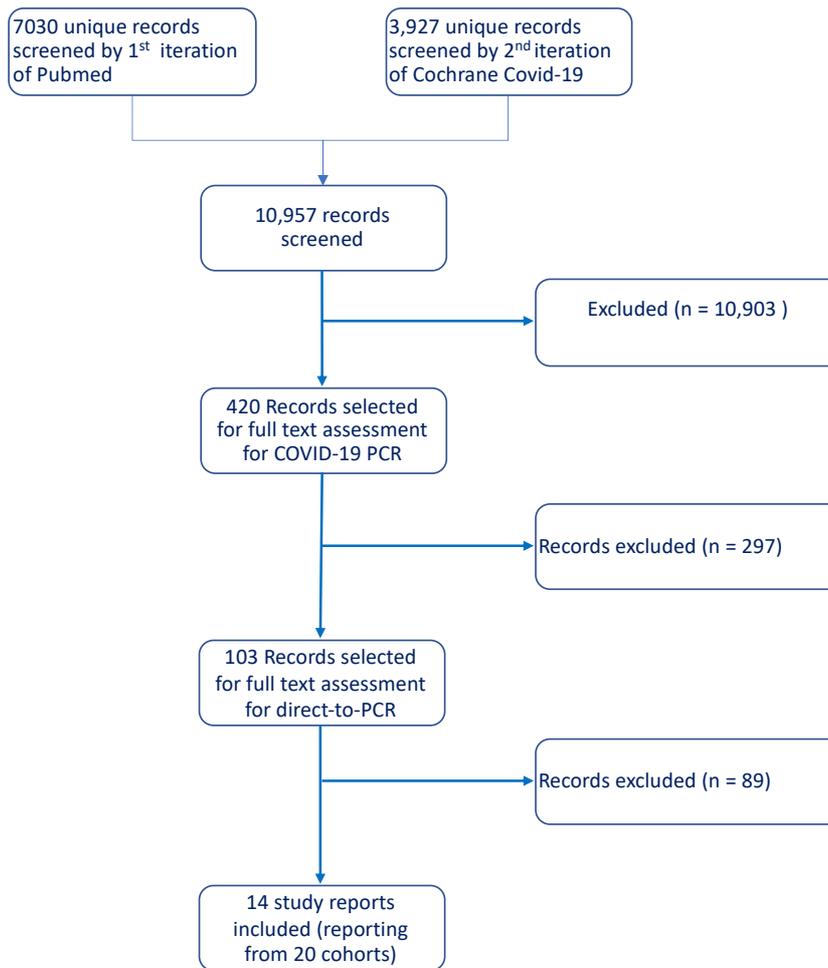


Figure 2. PRISMA flowchart

Included studies

Fourteen studies were included which reported 20 cohort datasets including 4460 patient samples and 1391 SARS-CoV-2 positive specimens.

Effects of interventions/results of the synthesis

Outcomes

10,957 unique records were identified and screened using a search string evaluation. 420 full-text reports and/or supplemental materials were assessed for inclusion. 14 studies reporting 20 datasets with 4593 patient samples (1391 positive) were included in the analysis. There were 4460 concordant and 133 discordant results as described in the contingency table below (**Table 3: Summary contingency table**).

	+ Central -	
+	1302	44
Direct		
-	89	3158

The overall agreement between the rapid direct PCR and standard centralised laboratory PCR was 97.10% with 93.60% positive percent agreement and 98.63% negative percent agreement and is summarized in Figure 3.

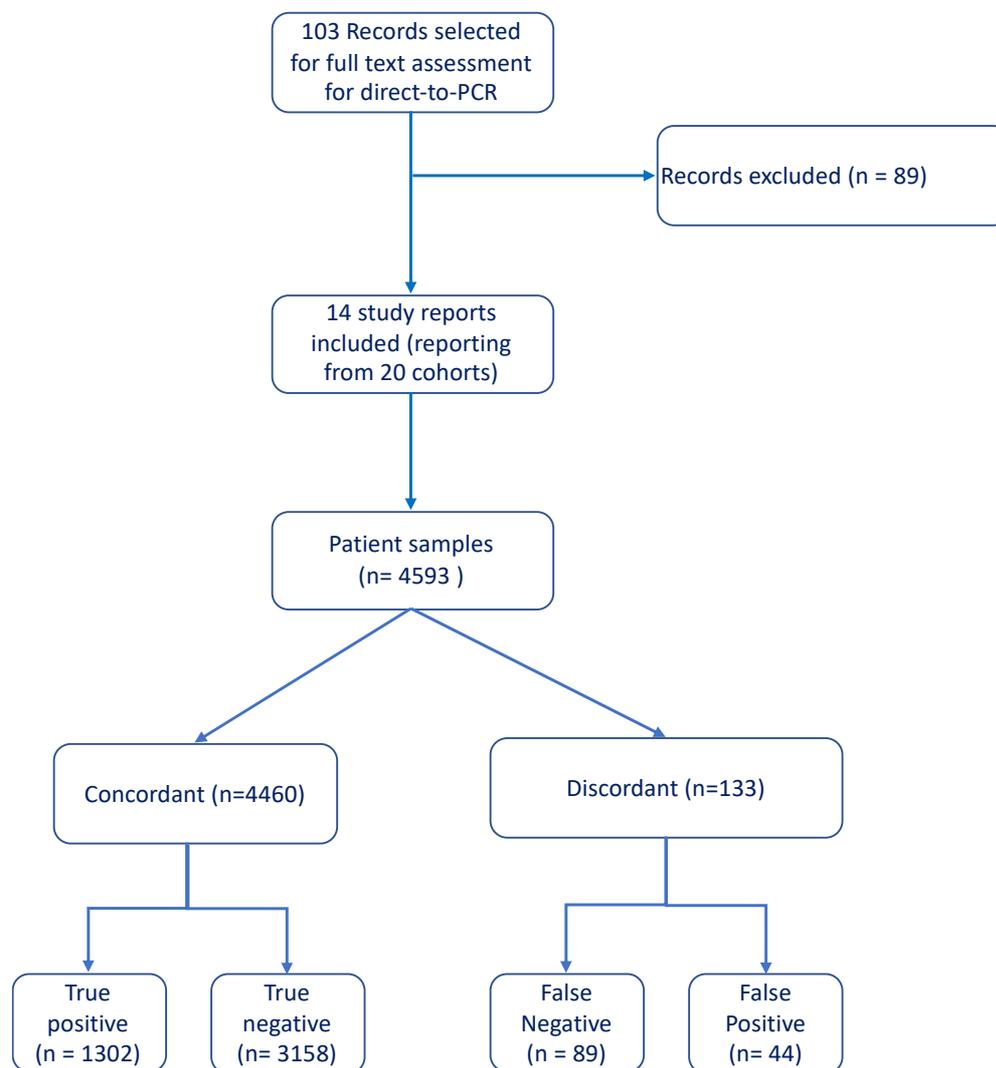


Figure 3. Summary of concordance

The results and outcomes for each study and are shown in table 1 below and an expanded analysis and references provided in the supplemental materials.

Table 4. Summary of study results

Name of study (3-17)	# Samples	# True Positive	# True Negative	# False Positive	# False Negative	PPA	NPA	OPA
Jørgensen et al. 2021	60	27	30	0	3	90.00%	100.00%	95.00%
Kellner et al. 2021	384	139	219	4	22	86.34%	98.21%	93.23%
Byrnes et al. 2021	246	82	150	0	14	85.42%	100.00%	94.31%
Zhen et al. 2020	104	51	53	0	0	100.00%	100.00%	100.00%

Bordi et al. 2020	278	99	171	8	0	100.00%	95.53%	97.12%
Lübke et al. 2020	90	74	0	1	15	83.15%	0.00%	82.22%
CICERO	1172	152	1017	2	1	99.35%	99.80%	99.74%
Bordi et al. 2020	41	21	16	4	0	100.00%	80.00%	90.24%
Miscio et al. 2020	266	63	203	0	0	100.00%	100.00%	100.00%
Fournier et al 2020	534	155	358	20	1	99.36%	94.71%	96.07%
Exsig NHS validation	483	132	341	0	10	92.96%	100.00%	97.93%
Clinical valuation of exsig	88	43	45	0	0	100.00%	100.00%	100.00%
PROMate TVG validation	759	221	512	5	21	91.32%	99.03%	96.57%
Clinical valuation of PROMate	88	43	43	0	2	95.56%	100.00%	97.73%
Totals:	4593	1302	3158	44	89	93.60%	98.63%	97.10%


Table 5. Summary of results by assay

Assay	Name of study	Number of samples	True Positive	True Negative	False Positive	False Negative	PPA	NPA	OPA
Simplexa™ COVID-19 Direct	Zhen et al. 2020	104	51	53	0	0	100.0%	100.0%	100.0%
	Bordi et al. 2020	278	99	171	8	0	100.0%	95.5%	97.1%
	Bordi et al. 2020	41	21	16	4	0	100.0%	80.0%	90.2%
	Total	423	171	240	12	0	100.0%	95.2%	97.2%
exsig® COVID-19 Direct	CICERO	1172	152	1017	2	1	99.3%	99.8%	99.7%
	Exsig NHS validation	483	132	341	0	10	93.0%	100.0%	97.9%
	Clinical valuation of exsig	88	43	45	0	0	100.0%	100.0%	100.0%
	Total	1743	327	1403	2	11	96.7%	99.9%	99.3%
PROMate® COVID-19	PROMate TVG validation	759	221	512	5	21	91.3%	99.0%	96.6%
	Clinical valuation of PROMate	88	43	43	0	2	95.6%	100.0%	97.7%
	Total	847	264	555	5	23	92.0%	99.1%	96.7%

Assessment of Heterogeneity

Heterogeneity between studies was examined by visually inspecting the forest plots of sensitivity and specificity (figure 4).

Figure 4. Forest plots of sensitivity and specificity

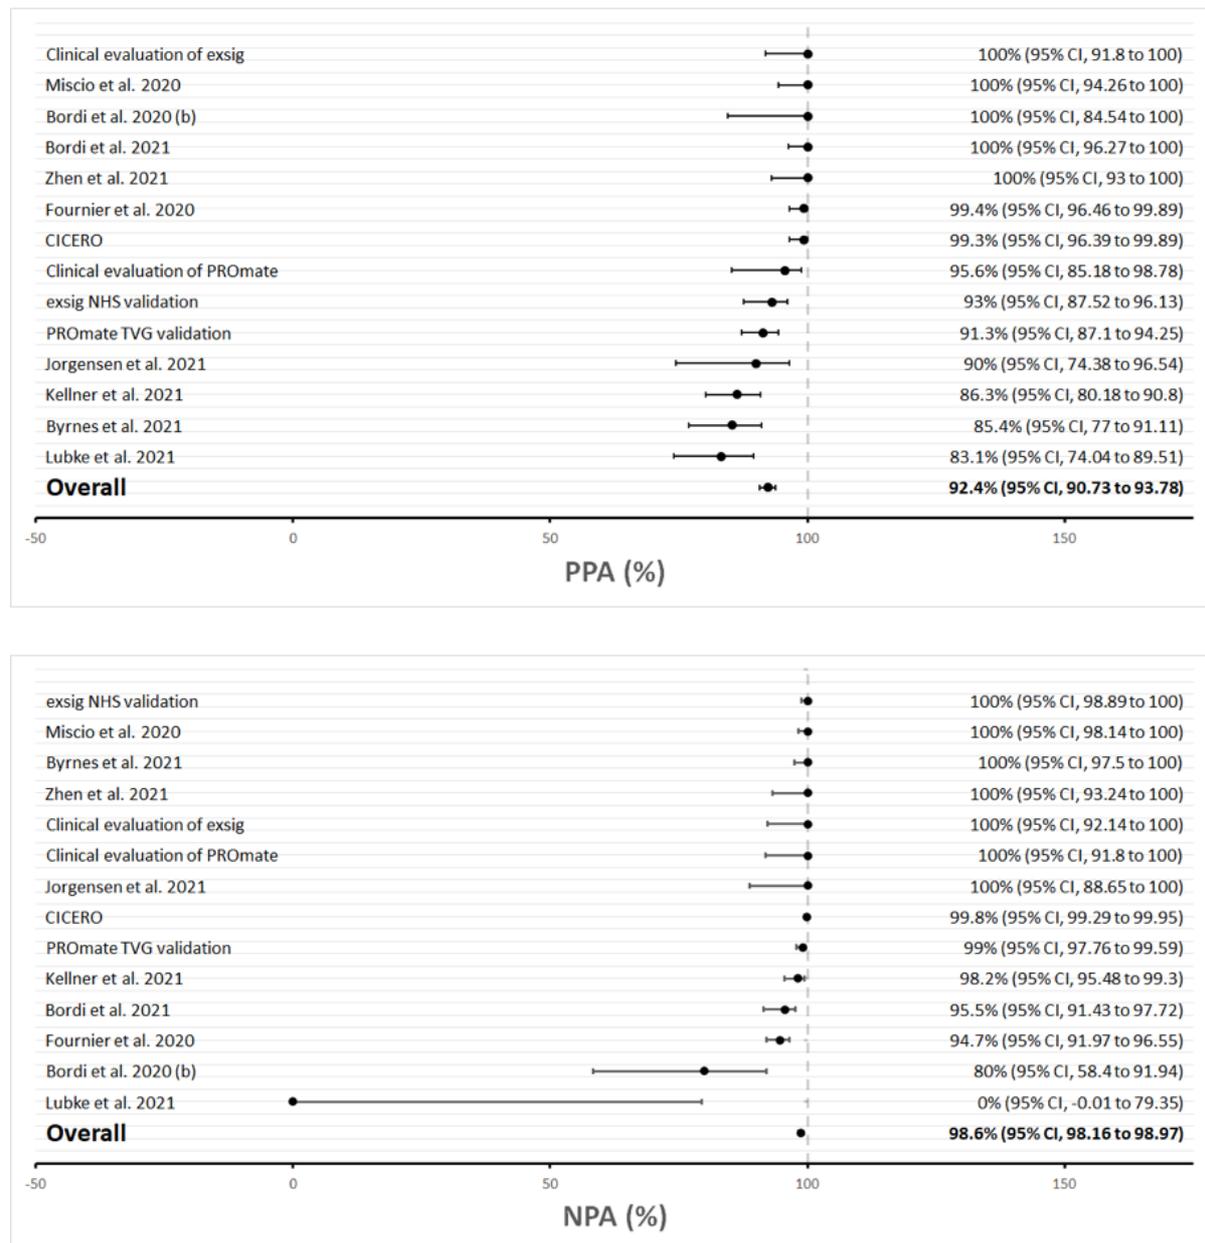

The overall agreement between the rapid direct PCR and standard centralised laboratory PCR was 97.1% with 93.60% positive percent agreement and 98.63% negative percent agreement. The Cohen's kappa statistical coefficient $k = 0.93$, indicating an almost perfect agreement and Youden Index = 0.92. These results show that direct-to-PCR assays perform equivalently to the standard centralised laboratory PCR systems for the diagnosis of SARS-CoV-2.

Discussion

Summary of main findings

Rapid direct-to-PCR systems further aim to reduce the speed of testing by combining rapid-PCR instruments with direct-to-PCR assays, to generate results in <2 hours. If sufficiently accurate, rapid tests returned within the same clinical encounter can facilitate timely decisions concerning the need for isolation and contact tracing activities¹ and create novel patient care pathways for the rapid diagnosis and treatment of COVID-19, and support infection prevention and control.

[Background and here]

This appears to be the first meta-analysis assessing the accuracy of rapid direct-to-PCR in the detection of SARS-CoV-2 and is the first iteration of this living review and will be updated in 3-6 months. In this meta-analysis 10,957 unique records were identified and screened using a search string evaluation, 420 full-text reports and/or supplemental materials were assessed for inclusion. This resulted in 14 studies reporting 20 data-sets with 4593 patient samples (1391 positive) included in the analysis.

Through this analysis, several potential sources of heterogeneity in the comparative evaluation methodology, whereby a new RT-PCR assay is compared with a reference RT-PCR assay were identified. Firstly, the direct-to-PCR reaction involves a dilution step whereas the more traditional RT-PCR involves a concentration step. In the dilution step, the quantity of nucleic acid in the sample is diluted potentially increases the likelihood of a false negative result. Conversely for the same viral load in an extracted PCR reaction, the concentration step concentrates or enriches the quantity of RNA potentially. Therefore, this could present a significant source of systematic bias. Furthermore, comparing assays with different gene targets adds another fundamental source of bias because detection of sub-genomic RNA may not be a suitable indicator of active replication/infection. Sub-genomic was found to have accumulated and remain detectable 17 days after infection.¹⁵ Therefore, the comparison of an assay that detects genomic RNA (ORF1ab) versus an assay detecting sub-genomic RNA (E-gene) may introduce a further systematic bias.

Nevertheless, overall agreement between the rapid direct PCR and standard centralised laboratory PCR was 97.1% with 93.60% positive percent agreement and 98.63% negative percent agreement. The Cohen's kappa statistical coefficient $k = 0.93$, indicating an almost perfect agreement and Youden Index = 0.92. These results show that direct-to-PCR assays perform equivalently to the gold standard centralised laboratory PCR systems for the diagnosis of SARS-CoV-2.

Authors' conclusions

This meta-analysis of the accuracy of rapid direct PCR for the diagnosis of SARS-CoV-2 included fourteen reports encompassing 21 datasets with a total of 3348 patient samples (1007 positive). The overall agreement between the rapid direct PCR and standard centralised laboratory PCR was 97.1% with 93.60% positive percent agreement and 98.63% negative percent agreement. The Cohen's kappa statistical coefficient $k = 0.93$, indicating an almost perfect agreement and Youden Index = 0.92. These results show that direct-to-PCR assays perform equivalently

to the standard centralised PCR systems for the diagnosis of SARS-CoV-2 and support the investigation of new rapid patient pathways for the detection and treatment of COVID-19

Declarations of Interest

The authors Stephen P. Kidd*, and J.E Martin* have no direct conflict of interest, JEM is principal investigator on the CICERO trial, funded by Novacyt. R.A. Trevor, S. Gripon, L. Koh, H. Chen, D. Borley and P. Oladimeji are employees of Novacyt group.

*joint senior authors

References

1. Dinnes J, Deeks JJ, Berhane S et al. Rapid, point-of-care antigen and molecular-based tests for diagnosis of SARS-CoV-2 infection. *Cochrane Database of Systematic Reviews*. 2021(3).
2. Page MJ, McKenzie JE, Higgins JP. Tools for assessing risk of reporting biases in studies and syntheses of studies: a systematic review. *BMJ open*. 2018 Mar 1;8(3):e019703.
3. Jørgensen RL, Pedersen MS, Chauhan AS, et al. An in-well direct lysis method for rapid detection of SARS-CoV-2 by real time RT-PCR in eSwab specimens. *Journal of Virological Methods*. 2021 Mar 1; 289:114062.
4. Kellner MJ, Matl M, Ross JJ et al. Head-to-head comparison of direct-input RT-PCR and RT-LAMP against RTqPCR on extracted RNA for rapid SARS-CoV-2 diagnostics. *medRxiv*. 2021 Jan 1.
5. Byrnes SA, Gallagher R, Steadman A, et al. Multiplexed and extraction-free amplification for simplified SARS-CoV-2 RT-PCR tests. *Analytical chemistry*. 2021 Feb 25;93(9):4160-5.
6. Zhen W, Manji R, Smith E, Berry GJ. Comparison of four molecular in vitro diagnostic assays for the detection of SARS-CoV-2 in nasopharyngeal specimens. *Journal of clinical microbiology*. 2020 Jul 23;58(8).
7. Bordi L, Piralla A, Lalle E et al. Rapid and sensitive detection of SARS-CoV-2 RNA using the Simplexa™ COVID-19 direct assay. *Journal of Clinical Virology*. 2020 Jul 1; 128:104416.
8. Lübke N, Senff T, Scherger S, et al. Extraction-free SARS-CoV-2 detection by rapid RT-qPCR universal for all primary respiratory materials. *Journal of Clinical Virology*. 2020 Sep 1;130: 104579.
9. COVID-19 in vitro diagnostic near-patient testing in Care Environments using a cluster Randomised Open-label trial design in an East London care home population (CICERO) : DATA ON FILE
10. Bordi L, Sberna G, Lalle E, et al. Frequency and duration of SARS-CoV-2 shedding in oral fluid samples assessed by a modified commercial rapid molecular assay. *Viruses*. 2020 Oct;12(10):1184.
11. Miscio L, Olivieri A, Labonia F et al. Evaluation of the diagnostic accuracy of a new point-of-care rapid test for SARS-CoV-2 virus detection. *Journal of translational medicine*. 2020 Dec;18(1):1-6.
12. Fitoussi F, Dupont R, Tonen-Wolyec S, Bélec L. Practicability and analytical performances of the novel VitaPCRTM SARS-CoV-2 Assay during the second wave of COVID-19 epidemic in France. *Journal of Medical Virology*. 2021 Mar 19.
13. NHS in-service evaluation of exsig COVID-19 direct assay (November 2020) - DATA ON FILE
14. Exsig Covid-19 direct evaluation (April 2021)- DATA ON FILE
15. Technical Validation of Primer Design Ltd PROMate™ COVID-19 Direct Workflow Solution IFU version 3.0 (published online February 2021) Doi: https://assets.publishing.service.gov.uk/government/uploads/system/uploads/attachment_data/file/957995/TVG_Report-PROMate.pdf
16. Covid-19 direct evaluation (April 2021)- DATA ON FILE
17. Alexandersen S, Chamings A, Bhatta TR. SARS-CoV-2 genomic and subgenomic RNAs in diagnostic samples are not an indicator of active replication. *Nature communications*. 2020 Nov 27;11(1):1-3.

Appendices

Appendix1 outlines the Direct-to-PCR assays that were analysed in this review

Ref	Author(s)	Samples (n)	True Pos	True Neg	False Pos	False Neg	PPA	NPA	OPA	Gene Targets	Direct to PCR assay	LoD	Comparator	Comparator Gene Targets	LOD Comparator
1	Jorgensen et al. 2021	60	27	30	0	3	90%	100%	95%	E gene	Research Assay	N.A.	Luna MM	E gene?	N.A.
2	Kellner et al. 2021	384	139	219	4	22	86%	98%	93%	N gene	Research Assay	N.A.	One -Step Quantitative RT-PCR System (ThermoFisher) and primer/probe (LightMix)	E gene	
3	Bynes et al. 2021	246	82	150	0	14	85%	100%	94%	N1 and N2	Research Assay	N.A.		N1 and N2	
4	Zhen et al. 2020	104	51	53	0	0	100%	100%	100%	ORF1ab and S gene	Simplexa™ COVID-19 Direct	S: 39 ± 23 Orf1ab: 602 ± 28 Final LOD: 39 ± 23 cp/ml	Modified CDC Assay, GenMark, Hologic	Modified CDC Assay (N1 and N2 genes), GenMark (N gene), Hologic (Orf1ab)	CDC: N1: 779±/± 27 ; N2: 356 ± 20 Final LOD: 779 ± 27 copies/ml Genmark: 1,000 cp/ml Hologic: 83 ± 36 cp/ml
5	Bordi et al. 2020	278	99	171	8	0	100%	96%	97%	ORF1ab and S gene	Simplexa™ COVID-19 Direct	3.2 (CI:2.9 to 3.8) log10 cp/ml for S; 3.2 (CI:2.9 to 3.7) log10 cp/ml for ORF1ab	Corman's Assay	RdRP and E gene	N.A.

Ref	Author(s)	Samples (n)	True Pos	True Neg	False Pos	False Neg	PPA	NPA	OPA	Gene Targets	Direct to PCR assay	LoD	Comparator	Comparator Gene Targets	LOD Comparator
6	Lübke et al. 2020	90	74	0	1	15	83%	0%	82%	E gene	PrimeDirect Probe (Research Assay)	N.A.	RNA-based RT-qPCR with the protocol by Corman and colleagues or by the ROCHE cobas® SARS-CoV-2 Test on the cobas® 6800 system (Roche).	ROCHE cobas® SARS-CoV-2 Test targets ORF1ab and E gene	N.A.
7	CICERO	1172	152	1017	2	1	99%	100%	100%	ORF1ab	exsig® COVID-19 Direct	1 copy/µl	ROCHE cobas® SARS-CoV-2 Test	ORF1ab and E gene	0.009 and 0.003 TCID ₅₀ /mL for SARS-CoV-2 (Target 1) and pan-Sarbecovirus (Target 2),
8	Bordi et al. 2020	41	21	16	4	0	100%	80%	90%	ORF1ab and S gene	Simplexa™ COVID-19 Direct	3.2 (CI: 2.9-3.8) log ₁₀ cp/ml for S and 3.2 log ₁₀ (CI: 2.9-3.7) log ₁₀ cp/ml for ORF1ab	Corman's Assay	RdRP, E and N gene	

Ref	Author(s)	Samples (n)	True Pos	True Neg	False Pos	False Neg	PPA	NPA	OPA	Gene Targets	Direct to PCR assay	LoD	Comparator	Comparator Gene Targets	LOD Comparator
9	Miscio et al. 2020	266	63	203	0	0	100%	100%	100%	N.A.	bKIT Virus Finder COVID-19 (Hyris Ltd)	LoD determined as the Ct threshold of 33	Abbott Kit: Real-Time SARS-CoV-2 (#09N77-095) and Roche Light Mix Modular but does not specify which samples were tested with either comparator	RdRP and N gene	
10	Fournier et al. 2020	534	155	358	20	1	99%	95%	96%	N gene	VitaPCR™ RT-PCR assay	N.A.	reference rRT-PCR	N gene	
11	Exsig NHS validation	483	132	341	0	10	93%	100%	98%	ORF1ab	exsig® COVID-19 Direct	1 copy/µl	Comparator assay only provided by 1 study centre (Cepheid Gene Xpert SARS CoV-2 Kit) while the other centres did not disclose comparator assays	Cepheid: E and N2 gene: Others does not specify	
12	Clinical valuation of exsig	88	43	45	0	0	100%	100%	100%	ORF1ab	exsig® COVID-19 Direct	1 copy/µl	genesig Covid-19 Assay (1 Gene)	ORF1ab	1 copy/µl

Ref	Author(s)	Samples (n)	True Pos	True Neg	False Pos	False Neg	PPA	NPA	OPA	Gene Targets	Direct to PCR assay	LoD	Comparator	Comparator Gene Targets	LOD Comparator
13	PROmate TVG validation	759	221	512	5	21	91%	99%	97%	ORF1ab	PROmate® COVID-19	0.96 copies/μl	Altona RealStar Dual target SARS-CoV-2, Hologic Panther TMA SARS-CoV-2, Novacyt Genesig HT and ROCHE cobas® SARS-CoV-2 Test. Discrepancy analysis assay: Cepheid Xpress SARS-CoV-2 and Novodiag SARS-CoV-2	Altona (S gene), Panther (ORF1ab), genesig HT 9(ORF1a), ROCHE (ORF1ab and E gene), Cepheid (E and N2 gene), Novodiag (ORF1ab and N genes)	
14	Clinical valuation of PROmate	88	43	43	0	2	96%	100%	98%	ORF1ab	PROmate® COVID-19	0.96 copies/μl	genesig Covid-19 Assay (1 Gene)	ORF1ab	1 copy/μl
Totals:		4593	1302	3158	44	89	94%	99%	97%						