

Augmenting gait in a population exhibiting foot drop with adaptive functional electrical stimulation

Jeremiah Robison, MS¹, Ren Gibbons, MS², Dean Achelis¹, Brinnae Bent, PhD², Doug Wajda, PhD³, Rebecca Webster MSPT, PhD¹

¹CIONIC Inc., San Francisco, CA

²Edge Analytics Inc., Campbell, CA

³Department of Health and Human Performance, Cleveland State University, Cleveland, OH

ABSTRACT

Objective

To investigate the effects of personalized, adaptive, current-steering functional electrical stimulation (FES) of the lower leg to improve gait in people with foot drop.

Design

A one-group, pre-test post-test study.

Setting

Two gait analysis centers.

Participants

Thirty-two participants exhibiting symptoms of foot drop.

Interventions

Adaptive, current-steering FES enables precise control over dorsiflexor and evtor muscles, allowing for personalized treatment to correct key foot drop characteristics including dorsiflexion at heel strike and ankle inversion during swing phase. All participants received adaptive FES of the dorsiflexors and evtors during back-to-back walking sets. Participants completed up to three walking sets of unstimulated walking (pre-test) followed by lower-leg stimulated walking (post-test).

Main Outcomes Measures

The primary outcome measures include ankle dorsiflexion at heel strike and mean ankle inversion during swing phase. Secondary outcome measures include foot angle at heel strike and single-side heel strike to toe strike time (heel-toe time).

Results

The differences in pre-test versus post-test primary and secondary outcome measures were statistically significant ($p < 0.0125$) within our cohort. With adaptive, current-steering FES, ankle dorsiflexion at heel strike increased an average 5.2° , and ankle inversion during swing phase was reduced by an average -3.6° , bringing the ankle to a more neutral position for stabilization.

Conclusion

Gait augmentation using adaptive, current-steering FES improved gait in a population exhibiting symptoms of foot drop. By significantly increasing ankle dorsiflexion at heel strike and decreasing ankle inversion during swing phase, adaptive FES enabled a more neutral ankle at heel strike, which is associated with greater ankle stability and decreased fall risk.

Keywords

Functional electrical stimulation, foot drop, gait analysis, rehabilitation, stroke, multiple sclerosis

Abbreviations

FES

Functional Electrical Stimulation

AFO

Ankle Foot Orthoses

IMU

Inertial Measurement Unit

CI

Confidence Interval

Introduction

Neurological disease or injury can significantly impact gait through reduced voluntary movement or spasticity, which can impede physical safety and reduce the ability to participate in activities of daily living, which can hinder community engagement and emotional well-being.

Foot drop describes difficulty lifting the front part of the foot and is commonly seen in adults with muscle weakness related to upper motor neuron disease or injury, including stroke survivors and individuals with multiple sclerosis^{1,2}. Specifically, foot drop negatively impacts gait through decreased voluntary ankle dorsiflexion and excessive ankle inversion³. Decreased dorsiflexion can result in lessened dynamic loading response⁴ and increased fall risk⁵. Excessive inversion can lead to lateral instabilities, stretching of lateral ankle structures, ankle sprains, and ultimately pain during weight acceptance⁶.

Foot drop severity can be quantitatively assessed with several kinematic metrics. The primary outcome metrics for this study are dorsiflexion at heel strike⁷ and mean inversion during swing phase⁸. The secondary outcome metrics are foot angle at heel strike and heel-toe time (single-side heel strike to toe strike time). Foot angle at heel strike has study relevance since lower foot angles can indicate decreased toe clearance during the swing phase of gait⁹. Similarly, heel rocker is a gait function that improves the fluidity of weight acceptance¹⁰, which is often diminished in individuals with foot drop. Heel-toe time is a method for approximating heel rocker function.

Various assistive technologies exist to address gait deviations in individuals with foot drop. These include orthoses such as AFOs, assistive devices such as canes and walkers, and functional electrical stimulation (FES) devices¹¹. FES devices improve gait by applying low amplitude electrical pulses to skeletal muscles to induce involuntary contraction to replace interrupted pathways from the central nervous system to peripheral neurons. Contrary to passive devices, FES provides dynamic stabilization and enables more normative movement of the ankle during gait¹².

FES gait augmentation systems offer numerous benefits over passive orthoses to individuals with impacted mobility¹¹. FES gait training has been shown to improve walking speed and duration compared to traditional orthotic gait devices¹³. FES has been linked to increased endurance^{14,15}, effective neural retraining¹⁶, and increased bone density^{17,18}. Despite these benefits, currently available FES systems have significant limitations: stimulation tuning for improved ankle dorsiflexion while maintaining balanced ankle eversion is challenging for fixed electrode devices¹⁹. Additionally, other FES devices lack adaptive personalized algorithms for fine-tuned temporal stimulation sequencing²⁰.

The Cionic Neural Sleeve is the first FES system that provides adaptive, multi-channel current-steering FES to enable precise control of the dorsiflexors and evertors (including the tibialis anterior and the peroneus longus). This enables the system to reduce key foot drop characteristics, including ankle dorsiflexion and inversion, and personalize treatment for foot drop.

The primary aim of this study was to investigate whether adaptive, current-steering FES of the lower leg improves gait in participants with foot drop, as measured by ankle dorsiflexion, ankle inversion, foot angle, and heel-toe time.

Methods

Participant recruitment

A total of 60 participants were assessed for eligibility. Study inclusion criteria specified participants must be an adult aged 18-70 living with a lower extremity impairment that makes walking difficult or uncomfortable; be capable of sitting, standing, and walking independently or with assistance; be able to walk at least 50 feet independently or with assistance; and be able to understand and follow basic instructions in English. Of those assessed, eight were excluded due to not meeting eligibility requirements, declining to participate, or other. Fifty-two were enrolled in the study. Of the enrollees, fourteen were lost to follow up due to scheduling logistics. Thirty-eight were allocated for data collection. Four of the allocated were excluded for insufficient endurance to complete the experimental protocol, and two were excluded due to equipment errors. The final analysis pool contained 32 subjects.

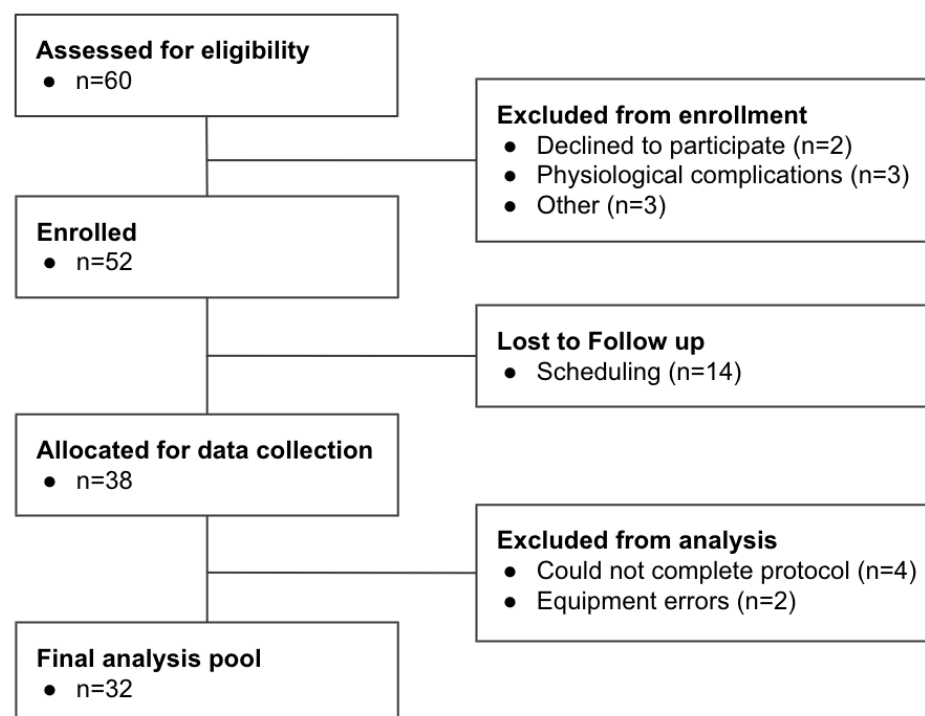


Figure 1. Flow chart on participant inclusion. Of 60 assessed for eligibility, 52 were enrolled. Thirty-eight of the enrollees were allocated for data collection, and 32 were included in the final pool. Reasons for exclusion from analysis include inability to complete protocol and equipment errors.

Ethical considerations

The present study was carried out according to the Declaration of Helsinki. Participation was voluntary and based on written informed consent from the participant. The study has been approved by the Institutional Review Board at Ethical & Independent Review Services (E&I 21039-01A) and the Institutional Review Board at Cleveland State University (IRB-FY2021-301).

Study design

The study design is a one-group, pre-test post-test study where we assessed the impact of FES relative to each participant's unstimulated gait in a pairwise fashion. All participants received adaptive FES to the dorsiflexors and evertors during up to three back-to-back walking sets.

Technology

In this study, we use the Cionic Neural Sleeve, an adaptive, current-steering FES device to stimulate dorsiflexors and evertors to improve ankle movement. The novel technology includes an array of FES gel electrodes placed on the anterolateral region of the impaired lower leg (Figure 2), corresponding with the atlas of the muscle motor points for the lower limb²¹. The frequency (Hz) and pulse width (μ s) of all electrodes are tunable. Additionally, the current intensity (mA) of each electrode in the array can be independently configured using a mobile application. This multi-channel current-steering allows for precision control of ankle movement in multiple planes. The sequencing of muscle stimulation is controlled by algorithms operating on data streamed from on-body sensors. Specifically, the algorithms use spatial orientation data to trigger muscle contraction and relaxation events that adapt to changes in gait speed.



Figure 2. Left: Cionic Neural Sleeve showing the configuration of the FES and EMG electrode arrays. Center: Cionic mobile application interface for setting FES parameters (frequency, pulsewidth, intensity) and current field steering. Right: Cionic Neural Sleeve on body.

Data collection

Prior to walking with FES, each participant underwent a standard seated FES configuration protocol facilitated by trained researchers to set stimulation parameters to achieve observable dorsiflexion (ideally exceeding 10°) with balanced eversion while maintaining participant comfort. Frequency and pulse width parameters were set to 40 Hz and 300 μ s, respectively, and intensity was increased until the desired ankle movement was achieved. Frequency and pulse width could also be tuned in increments of 5 Hz and 100 μ s as needed for comfort or efficacy. FES configuration was completed using the Cionic mobile application. Each participant gained familiarity with stimulated gait by traversing a 40-foot walkway as a warmup. They walked with their typical assistive devices, if applicable, excluding AFOs.

Next, each participant alternated between unstimulated (noFES) walking collection of their typical gait and stimulated (FES) walking collection. Data was collected from the Cionic Neural Sleeve using the following sensors: Bosch Sensortec inertial measurement units (IMUs) placed on the thigh, shank, and foot to reconstruct the leg's spatial orientation and three foot pressure sensor pads sampled using an analog-to-digital converter (ADS1298CZXGT, Texas Instruments) in the shoe for gait event detection. IMUs were calibrated prior to each participant's collections. For the stimulated collections, the dorsiflexors were stimulated to maintain toe clearance during swing phase and improve heel strike, and evertors to achieve neutral ankle at heel strike and loading response. Unstimulated and stimulated collections were performed back-to-back up to three times (six total collections) to directly quantify the impact of FES. Each collection consisted of walking across the walkway, turning around, and walking back to the starting point. Time intervals corresponding to the turn around were identified via manual inspection of kinematics data and were removed from the analysis. The first two steps and last step for each length of the walkway were removed from the analysis. Pressure sensor data was automatically labeled and manually inspected to extract heel strike, toe strike, and toe off events.

Statistical analyses

Based on our statistical power analysis, we required eighteen or more participants to achieve 80% power to reject the null hypothesis which states there is no difference between pre-test (noFES) and post-test (FES) conditions in a pairwise comparison ($\alpha = 0.05$). We selected an effect size of 0.7 for the power analysis based on a previous study of FES impact on post-stroke participants²².

In this analysis, we examined whether the impact of FES on gait is statistically significant relative to unstimulated gait by pairwise comparison. For each metric, we averaged each participant's metric values across steps for both noFES and FES walking. Each metric's final analysis pool contained 32 noFES and 32 FES samples. The Shapiro-Wilk test for normality²³

was used to assess the assumption of normality and paired t-tests were used to statistically compare noFES and FES foot drop metrics if the assumption for normality was met (all metrics except foot angle at heel strike). If the normality assumption was not met, the Wilcoxon signed rank test was used as an alternative to the paired t-test (this was the case for foot angle at heel strike). Bonferroni multiple hypothesis correction was performed (four metrics tested), and our corrected significance level for comparison was 0.0125 (0.05 divided by the four hypotheses tested). We also report the 95% confidence interval for the differences between FES and noFES foot drop metrics.

Results

Current-steering FES enables precise control over muscles to personalize the balance between dorsiflexion and inversion. The primary outcomes of this study were dorsiflexion at heel strike and inversion during swing phase, as these metrics are directly related to fall risk and ankle stabilization, respectively. Our secondary outcomes of this study include foot angle at heel strike and heel-toe time which also correlate to gait stability, dynamic loading response, and improved rocker²³.

Participant demographics

The final analysis pool was split across 32 participants aged 61.1 ± 10.9 living near San Francisco and Cleveland. The subjects included 18 females and 14 males. All subjects had a diagnosis of neurological disease or injury: 20 were post-stroke, eight had multiple sclerosis, two had a spinal cord injury, one had cerebral palsy, and one had idiopathic foot drop. All exhibited symptoms of foot drop. The average stimulation parameters across participants included an amplitude of 44 ± 11 mA, frequency of 38 ± 14 Hz, and a pulse duration of 306 ± 51 μ s.

Primary outcomes

The impacts of FES on dorsiflexion across 32 participants exhibiting symptoms of foot drop are shown in Figure 3A. The kinematics profile shows average dorsiflexion throughout the gait cycle for all participants, and the shaded region shows the standard deviation. Zero percent corresponds to heel strike. Additionally, the participants' baseline noFES kinematics showing symptoms of foot drop are in orange while Cionic FES show the impact of gait assist in blue. We observed that the primary impact of FES on dorsiflexion occurs at heel strike and during swing phase (approximately to 65-100% of gait), and that dorsiflexion at heel strike is increased by an average of 5.2° (CI[3.5° , 6.8°]) with statistical significance (p -value= $7e-5$). The average increase of 5.2° is greater than the minimal clinically important difference of 4.9° as defined by the Clinical Practice Guideline for the Use of Ankle-Foot Orthoses and Functional Electrical Stimulation Post Stroke²⁴. All but one participant showed increased dorsiflexion at heel strike; the biggest observed increase from a participant was an average of 14.6° , while one decreased by -1.6° .

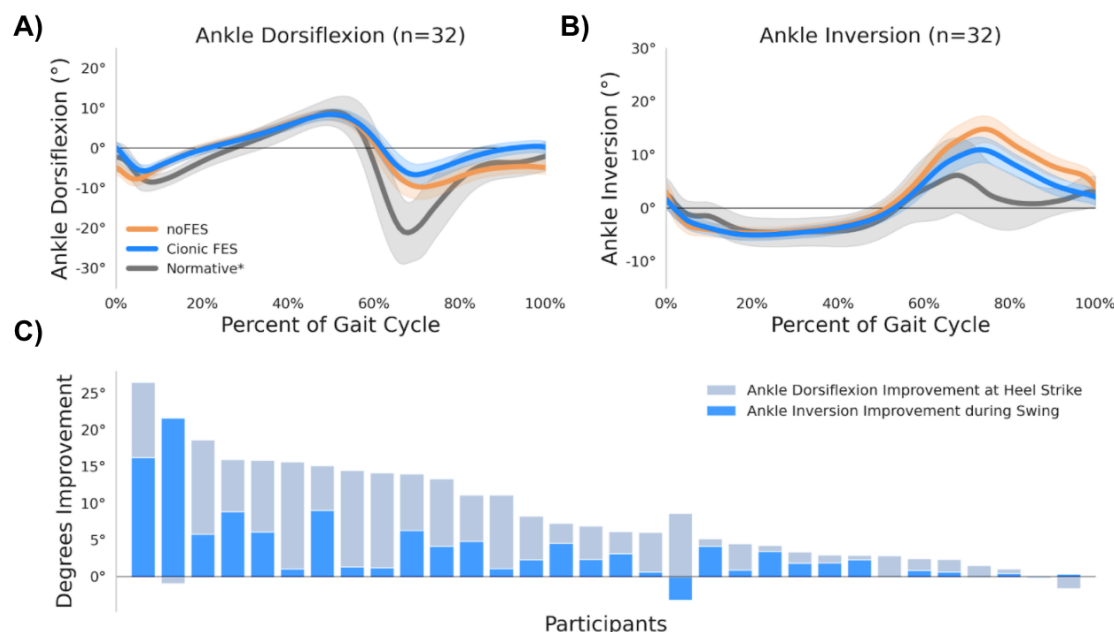


Figure 3. (A) Ankle dorsiflexion gait profiles averaged over the 32 participants walking with Cionic FES (blue profile) and without (orange profile). The gait cycle profile is represented as a percent, where 0% occurs at heel strike. The solid lines represent the cohort average, and the shaded intervals are \pm one standard deviation. (B) Ankle inversion gait profiles averaged over the 32 participants with Cionic FES (blue) and without (orange). (C) Stacked degrees of dorsiflexion improvement (gray bar) and inversion improvement (blue bar) for each participant. All participants but one showed a net improvement across both primary outcomes. *The gray normative profile was determined from the typical walking gait of eleven normative participants. This was a sample of convenience conducted on Cionic employees with no known gait impairments. Normative participant data was collected under IRB oversight and consisted of 11 participants (10 male, 1 female) with age range [24-53].

In addition to decreased dorsiflexion, many of the 32 participants also exhibit excessive ankle inversion as shown in Figure 3B. Excessive inversion is especially apparent for noFES during the swing phase. Evertor FES is configured to reduce ankle inversion during swing phase through loading response (Figure 3B) as this increases lateral loading response stability. We show an improved outcome by reducing mean inversion during the swing phase by an average of -3.6° (CI[-5.3°, -1.8°], p-value=3e-4). The largest observed decrease was an average of -21.6° . In total 88% of participants showed a positive improvement to ankle inversion during swing.

Figure 3C shows the stacked degrees of improvement for dorsiflexion and inversion for each participant, providing a more comprehensive picture of the impact of gait assist across multiple movements. Some participants exhibit large improvements to inversion due to high baseline inversion, while others show higher dorsiflexion improvement relative to inversion. All participants but three showed an improvement in both dorsiflexion and inversion, and all but one showed net improvement across both primary metric outcomes.

Secondary outcomes

We observed an average of 5.5° (CI[3.9° , 7.0°]) increase in foot angle at heel strike (p-value= $9e-7$). Heel-toe time increased by an average of 3.4% of gait (CI[1.9%, 4.8%], p-value= $4e-5$). After FES treatment, average foot angle at heel strike and heel-toe time were closer to the normative average. With dorsiflexor stimulation, foot angle increased in all participants except one, whose foot angle decreased by -0.4° . The largest FES-driven increase in foot angle was 15.8° . Additionally, stimulated gait resulted in increased heel-toe time in all but three participants, who decreased by no more than 1.8%. The participant with the greatest increase in heel-toe time showed a 17.5% increase.

Discussion

This study aimed to evaluate the effects of adaptive, multi-channel current-steering FES on gait in a population exhibiting foot drop. We demonstrated statistically significant improved gait in 32 participants exhibiting symptoms of foot drop due to neurological disorders. On average, these participants showed a 5.2° increase in dorsiflexion at heel strike and a 3.6° degree reduction in ankle inversion during swing phase. Together, this brings the ankle into a more stable, neutral position, which is associated with decreased fall risk⁵. The increase in dorsiflexion also resulted in a 5.5° increase in foot angle at heel strike which correlates to better foot clearance, and an increase in heel-toe time of 3.4% of the gait cycle has links to more dynamic loading response.

Neurological disease or injury can significantly impact gait, impeding physical safety and reducing the ability to participate in activities of daily living, which hinders community engagement and emotional well-being. Foot drop, a major inhibitor of mobility and a contributor to fall risk, is commonly seen in people with multiple sclerosis, post stroke, or other neurological conditions. Existing solutions for gait correction of foot drop include passive devices and FES systems, which stimulate skeletal muscles to restore motor function¹¹. FES provides dynamic stabilization, enabling movement while improving stability. While FES systems show enormous potential for gait improvements^{25,26}, current marketed products have limited capabilities for real-life mobility enhancements^{19,20}. Given the large number of people living with mobility impairments and the significant accessibility challenges and financial burdens they face²⁷, it is critically important to find solutions that address the shortcomings of current assistive gait devices.

The Cionic Neural Sleeve FES system used in this study utilizes adaptive current-steering to enable precise control over the dorsiflexors and evertors. Current-steering allows for personalization of the balance between increased dorsiflexion and reduced ankle inversion, leading to a more neutral ankle position at heel strike in order to reduce fall risk. While many FES solutions that enable personalized control of stimulation are available only in the clinical setting, the Cionic Neural Sleeve is available for at-home use, extending the applications of FES to include improved daily mobility and remote rehabilitation.

Study Limitations

This study did not include the collection of certain traditional gait analysis metrics including spatial measures like gait speed and stride length as we relied solely on the on-body device for all data collection and metric extraction. Additionally, we were not able to compare FES treatment impacts relative to standard of care, i.e. AFO, in a randomized control trial. An RCT remains a future research study.

Conclusions

The ability to reduce foot drop, which is a major inhibitor of mobility and a contributor to fall risk, would provide great value to those with impaired gait. This is the first study evaluating the effects of adaptive, current-steering stimulation from the Cionic Neural Sleeve on gait in patients exhibiting symptoms of foot drop. Precise control over the dorsiflexor and evtor muscles results in statistically significant improvements to ankle movement, including increased dorsiflexion and decreased inversion, which can stabilize the ankle and decrease fall risk.

References

1. Stewart JD. Foot drop: where, why and what to do? *Pract Neurol*. 2008;8(3):158-169. doi:10.1136/jnnp.2008.149393
2. Foot drop. Physiopedia. Accessed March 29, 2022. https://www.physio-pedia.com/Foot_drop
3. Stevens F, Weerkamp NJ, Cals JWL. Foot drop. *BMJ*. 2015;350:h1736. doi:10.1136/bmj.h1736
4. Alam M, Choudhury IA, Mamat AB. Mechanism and Design Analysis of Articulated Ankle Foot Orthoses for Drop-Foot. *Sci World J*. 2014;2014:867869. doi:10.1155/2014/867869
5. Foot Drop Information Page | National Institute of Neurological Disorders and Stroke. Accessed March 29, 2022. <https://www.ninds.nih.gov/Disorders/All-Disorders/Foot-Drop-Information-Page>
6. Morrison KE, Kaminski TW. Foot Characteristics in Association With Inversion Ankle Injury. *J Athl Train*. 2007;42(1):135-142.
7. Kesar TM, Perumal R, Jancosko A, et al. Novel Patterns of Functional Electrical Stimulation Have an Immediate Effect on Dorsiflexor Muscle Function During Gait for People Poststroke. *Phys Ther*. 2010;90(1):55-66. doi:10.2522/ptj.20090140
8. Pierrynowski MR, Smith SB. Rear Foot Inversion/Eversion During Gait Relative to the Subtalar Joint Neutral Position. *Foot Ankle Int*. 1996;17(7):406-412. doi:10.1177/107110079601700709
9. Nori SL, Stretanski MF. Foot Drop. In: *StatPearls*. StatPearls Publishing; 2022. Accessed March 29, 2022. <http://www.ncbi.nlm.nih.gov/books/NBK554393/>
10. Daryabor A, Aminian G, Arazpour M, Baniasad M, Yamamoto S. The effects of ankle-foot orthoses with plantar flexion stop and plantar flexion resistance using rocker-sole shoes on stroke gait: A randomized-controlled trial. *Turk J Phys Med Rehabil*. 2021;67(4):449-461. doi:10.5606/tftrd.2021.6448
11. York G, Chakrabarty S. A survey on foot drop and functional electrical stimulation. *Int J Intell Robot Appl*. 2019;3(1):4-10. doi:10.1007/s41315-019-00088-1
12. Springer S, Khamis S. Effects of functional electrical stimulation on gait in people with

- multiple sclerosis - A systematic review. *Mult Scler Relat Disord*. 2017;13:4-12. doi:10.1016/j.msard.2017.01.010
13. Nightingale EJ, Raymond J, Middleton JW, Crosbie J, Davis GM. Benefits of FES gait in a spinal cord injured population. *Spinal Cord*. 2007;45(10):646-657. doi:10.1038/sj.sc.3102101
14. Hakansson NA, Hull ML. Muscle stimulation waveform timing patterns for upper and lower leg muscle groups to increase muscular endurance in functional electrical stimulation pedaling using a forward dynamic model. *IEEE Trans Biomed Eng*. 2009;56(9):2263-2270. doi:10.1109/TBME.2009.2020175
15. Schardong J, Kuinchtner GC, Sbruzzi G, Plentz RDM, Silva AMV da. Functional electrical stimulation improves muscle strength and endurance in patients after cardiac surgery: a randomized controlled trial. *Braz J Phys Ther*. 2017;21(4):268-273. doi:10.1016/j.bjpt.2017.05.004
16. Kapadia N, Moineau B, Popovic MR. Functional Electrical Stimulation Therapy for Retraining Reaching and Grasping After Spinal Cord Injury and Stroke. *Front Neurosci*. 2020;14:718. doi:10.3389/fnins.2020.00718
17. Frotzler A, Coupaud S, Perret C, et al. High-volume FES-cycling partially reverses bone loss in people with chronic spinal cord injury. *Bone*. 2008;43(1):169-176. doi:10.1016/j.bone.2008.03.004
18. Lauer RT, Smith BT, Mulcahey MJ, Betz RR, Johnston TE. Effects of cycling and/or electrical stimulation on bone mineral density in children with spinal cord injury. *Spinal Cord*. 2011;49(8):917-923. doi:10.1038/sc.2011.19
19. Seel T, Laidig D, Valtin M, Werner C, Raisch J, Schauer T. Feedback control of foot eversion in the adaptive peroneal stimulator. In: *22nd Mediterranean Conference on Control and Automation*. ; 2014:1482-1487. doi:10.1109/MED.2014.6961585
20. Marquez-Chin C, Popovic MR. Functional electrical stimulation therapy for restoration of motor function after spinal cord injury and stroke: a review. *Biomed Eng OnLine*. 2020;19(1):34. doi:10.1186/s12938-020-00773-4
21. Botter A, Oprandi G, Lanfranco F, Allasia S, Maffiuletti NA, Minetto MA. Atlas of the muscle motor points for the lower limb: implications for electrical stimulation procedures and electrode positioning. *Eur J Appl Physiol*. 2011;111(10):2461. doi:10.1007/s00421-011-2093-y
22. Vafadar AK, Côté JN, Archambault PS. Effectiveness of Functional Electrical Stimulation in Improving Clinical Outcomes in the Upper Arm following Stroke: A Systematic Review and Meta-Analysis. *BioMed Res Int*. 2015;2015:e729768. doi:10.1155/2015/729768
23. SHAPIRO SS, WILK MB. An analysis of variance test for normality (complete samples)†. *Biometrika*. 1965;52(3-4):591-611. doi:10.1093/biomet/52.3-4.591
24. Johnston TE, Keller S, Denzer-Weiler C, Brown L. A Clinical Practice Guideline for the Use of Ankle-Foot Orthoses and Functional Electrical Stimulation Post-Stroke. *J Neurol Phys Ther JNPT*. 2021;45(2):112-196. doi:10.1097/NPT.0000000000000347
25. Tan Z, Liu H, Yan T, et al. The Effectiveness of Functional Electrical Stimulation Based on a Normal Gait Pattern on Subjects with Early Stroke: A Randomized Controlled Trial. *BioMed Res Int*. 2014;2014:545408. doi:10.1155/2014/545408
26. Yan T, Hui-Chan CWY, Li LSW. Functional Electrical Stimulation Improves Motor Recovery of the Lower Extremity and Walking Ability of Subjects With First Acute Stroke. *Stroke*. 2005;36(1):80-85. doi:10.1161/01.STR.0000149623.24906.63
27. Kabiri M, Brauer M, Shafrin J, Sullivan J, Gill TM, Goldman DP. Long-Term Health and Economic Value of Improved Mobility among Older Adults in the United States. *Value Health*. 2018;21(7):792-798. doi:10.1016/j.jval.2017.12.021