

## Supplemental Information

**Table S1.** Descriptive statistics and percentiles of flame-retardant<sup>a</sup> measurements for firefighters (n= 86) and office workers (n= 84)

Chemical	Group	LOD	DF%	GM (GSD)	Percentiles			
					25th	50th	75th	95th
<b>BCEP</b>								
	Firefighter	0.1	78	0.85 (5.74)	0.23	1.22	3.98	8.51
	Office worker	0.1	39	<LOD	<LOD	<LOD	0.485	3.31
<b>BDCPP</b>								
	Firefighter	0.2	100	4.08 (4.53)	1.30	5.37	13.3	32.22
	Office worker	0.2	90	0.96 (3.99)	<LOD	0.92	2.3425	8.72
<b>DBuP</b>								
	Firefighter	0.1	83	0.41 (3.92)	0.15	0.495	1.2575	3.04
	Office worker	0.1	29	<LOD	<LOD	<LOD	0.1275	0.56
<b>BDzP</b>								
	Firefighter	0.2	7	<LOD	<LOD	<LOD	<LOD	0.22
	Office worker	0.2	0	<LOD	<LOD	<LOD	<LOD	<LOD
<b>DoCP</b>								
	Firefighter	0.1	9	<LOD	<LOD	<LOD	<LOD	0.15
	Office worker	0.1	1	<LOD	<LOD	<LOD	<LOD	<LOD
<b>DpCP</b>								
	Firefighter	0.1	41	<LOD	<LOD	<LOD	0.2275	0.45
	Office worker	0.1	17	<LOD	<LOD	<LOD	<LOD	0.20
<b>TBBA</b>								
	Firefighter	0.2	24	<LOD	<LOD	<LOD	<LOD	0.42
	Office worker	0.2	8	<LOD	<LOD	<LOD	<LOD	0.24
<b>TBBPA</b>								
	Firefighter	0.2	45	<LOD	<LOD	<LOD	0.41	0.96
	Office worker	0.2	42	<LOD	<LOD	<LOD	0.29	0.64


Abbreviations: LOD = Limit of Detection; DF = Detection Frequency; GM = Geometric mean; GSD = geometric standard deviation

<sup>a</sup>2,2',4,4'-Tetrabromodiphenyl ether (OH-BDE 47) and 1,3,5-Tribromo-2-(2,4-dibromophenoxy)benzene (OH-BDE 100) were also quantified but not detected in participant's samples.

**Table S2.**  $\beta$ (95%CI) and percent change (95% confidence intervals) in TSH levels for each doubling of exposure of continuous BDCPP, BCEP and DBuP in the full cohort in adjusted<sup>a</sup> OLS regression models

	<b>Model</b>	<b><math>\beta</math>(95%CI)</b>	<b>Percent change (95%CI)</b>
Full cohort			
	BDCPP	-0.006 (-0.110,0.098)	-0.408 (-7.323,7.024)
	BCEP	-0.069 (-0.161,0.024)	-4.657 (-10.572,1.650)
	DBuP	-0.015 (-0.137,0.107)	-1.033 (-9.035,7.673)
Firefighters			
	BDCPP	0.050 (-0.150,0.251)	3.548 (-9.875,18.972)
	BCEP	-0.127 (-0.297,0.043)	-8.418 (-18.610,3.049)
	DBuP	0.018 (-0.195,0.231)	1.257 (-12.658,17.388)
Office workers <sup>b</sup>			
	BDCPP	-0.022 (-0.141,0.098)	-1.491 (-9.325,7.020)

<sup>a</sup> Models adjusted for age and log(creatinine) values below LOD replaced with LOD/sqrt(2); <sup>b</sup> Among office workers only BDCPP had DF >70% to use in linear models.

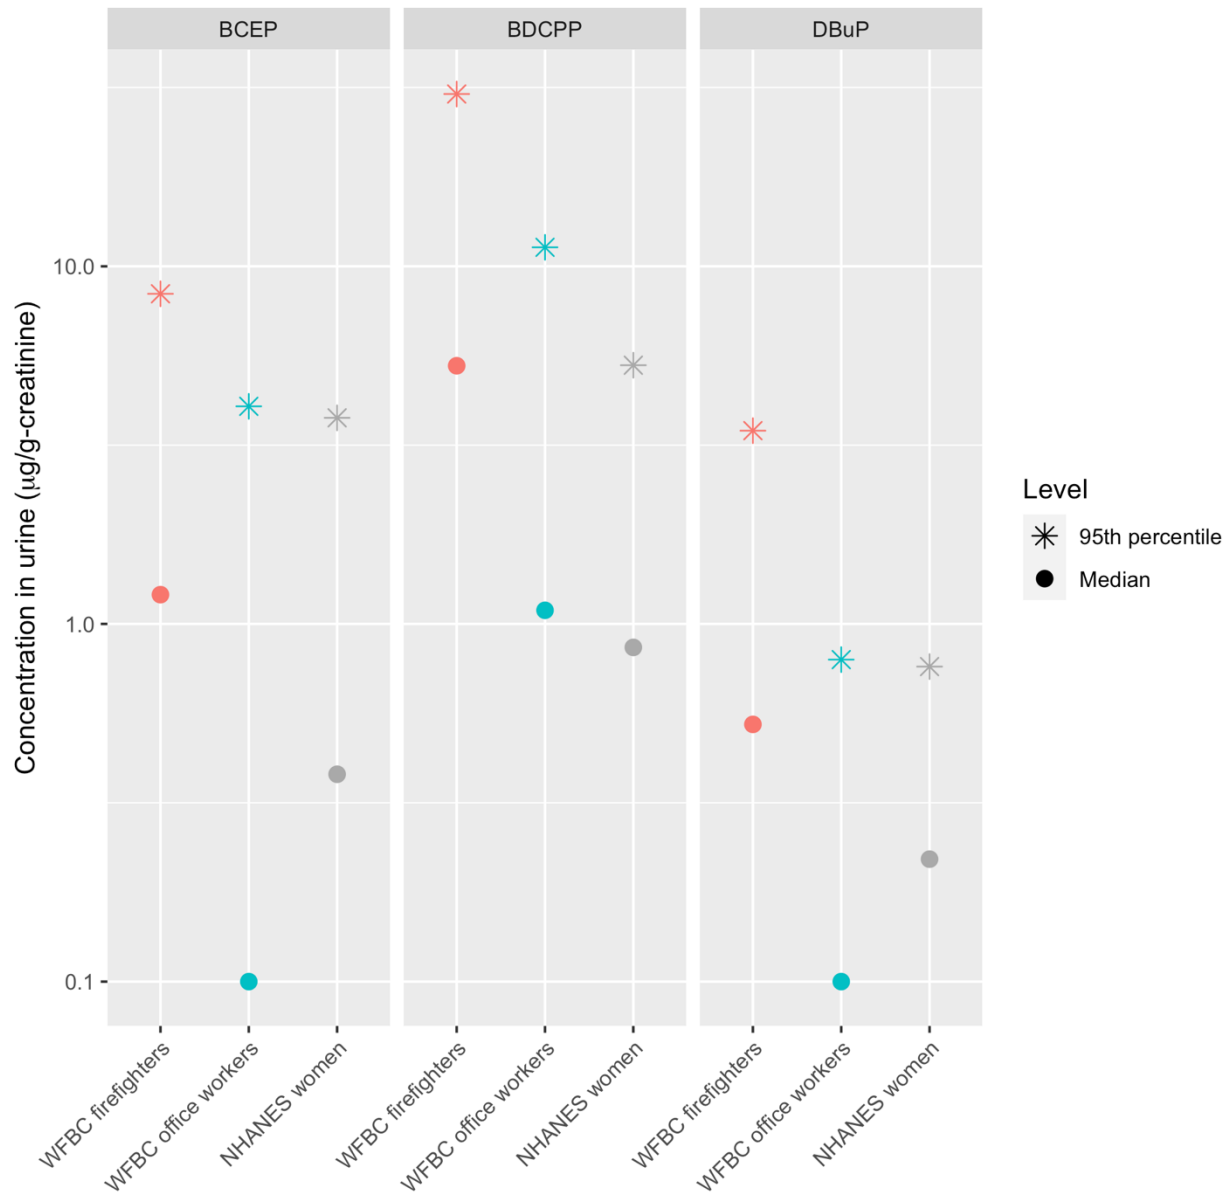

**Figure S1.** Median and 95th percentiles of flame retardants measured in urine ( $\mu\text{g/g-creatinine}$ ) from 2014-2015 WFBC firefighters and office workers compared to 2013-2014 NHANES adult women (ages 18 to 65) for compounds with at 70% DF among firefighters of the WFBC.