

Pool_raw_data


A	B	CTRPP	D	E	F	G	H	I	J	K	L	M	N	O	P	Q	R	S	T	U	V	W	X	Y	Z	AA	AB	AC	AD	AE	AF	AG	AH	AI	AJ	
Pool name	Original test date	Sample 1				cut-off N2	cut-off RPP30	Original test date	Sample 2				cut-off N2	cut-off RPP30	Original test date	Sample 3				cut-off N2	cut-off RPP30	Original test date	Sample 4				cut-off N2	cut-off RPP30	Original test date	Pool				cut-off N2	cut-off RPP30	
		Ct _{RPP}	Ct _{N2}	Ct _{E1}	Ct _{S6}				Ct _{RPP}	Ct _{N2}	Ct _{E1}	Ct _{S6}				Ct _{RPP}	Ct _{N2}	Ct _{E1}	Ct _{S6}				Ct _{RPP}	Ct _{N2}	Ct _{E1}	Ct _{S6}				Ct _{RPP}	Ct _{N2}	Ct _{E1}	Ct _{S6}			Ct _{RPP}
1N	29.65	N/A	N/A	N/A	34.78	35.37			30.66	N/A	N/A	N/A	34.78	35.37		26.43	N/A	N/A	44.16	34.78	35.37		23.62	N/A	N/A	41.22	34.78	35.37		27.49	27.49	N/A	N/A	35.45	36.50	
2N	32.04	N/A	N/A	N/A	34.78	35.37			29.48	38.87	N/A	N/A	34.78	35.37		27.93	39.49	N/A	42.52	34.78	35.37		28.55	N/A	N/A	N/A	34.78	35.37		28.20	43.22	N/A	N/A	38.33	35.45	36.50
3N	29.14	N/A	N/A	N/A	34.78	35.37			30.17	44.61	N/A	N/A	34.78	35.37		29.06	N/A	N/A	N/A	34.78	35.37		29.13	N/A	N/A	37.27	34.78	35.37		28.99	N/A	N/A	N/A	35.45	36.50	
4N	29.08	43.23	N/A	N/A	34.78	35.37			28.23	N/A	N/A	N/A	40.97	34.78	35.37		31.01	N/A	N/A	N/A	34.78	35.37		29.73	N/A	N/A	41.21	34.78	35.37		29.10	N/A	N/A	44.81	35.45	36.50
5N	28.40	N/A	43.83	43.58	34.78	35.37			29.67	N/A	N/A	40.24	34.78	35.37		29.14	N/A	N/A	N/A	34.78	35.37		29.15	N/A	N/A	38.58	34.78	35.37		28.54	N/A	N/A	37.38	35.45	36.50	
6N	32.08	N/A	N/A	N/A	34.78	35.37			30.35	N/A	N/A	40.00	34.78	35.37		29.44	38.40	40.34	N/A	34.78	35.37		29.45	N/A	N/A	41.71	34.86	34.75		29.97	N/A	N/A	N/A	35.45	36.50	
7N	29.17	N/A	N/A	N/A	34.86	34.75			30.81	N/A	N/A	N/A	34.86	34.75		29.33	N/A	N/A	N/A	34.86	34.75		30.38	N/A	37.10	39.72	34.86	34.75		29.28	38.82	N/A	N/A	35.45	36.50	
8N	27.52	N/A	43.27	N/A	34.86	34.75			30.64	N/A	N/A	N/A	34.86	34.75		27.81	N/A	N/A	40.70	34.86	34.75		28.70	N/A	N/A	40.85	34.86	34.75		29.26	N/A	N/A	N/A	35.45	36.50	
9N	30.52	N/A	N/A	N/A	34.86	34.75			30.88	N/A	N/A	N/A	34.86	34.75		30.29	37.16	N/A	N/A	34.86	34.75		31.64	N/A	N/A	N/A	34.86	34.75		29.84	N/A	N/A	40.30	35.45	36.50	
10N	28.02	N/A	N/A	N/A	34.86	34.75			28.38	N/A	N/A	43.41	34.86	34.75		29.17	N/A	N/A	N/A	34.86	34.75		31.14	N/A	N/A	40.94	34.86	34.75		28.10	N/A	N/A	37.62	35.45	36.50	
11N	27.38	N/A	N/A	N/A	34.78	35.37			31.39	N/A	N/A	N/A	34.86	34.75		29.46	N/A	N/A	N/A	34.86	34.75		29.62	36.24	37.70	41.67	34.86	34.75		28.37	N/A	N/A	43.20	35.45	36.50	
12N	31.82	N/A	37.02	N/A	34.86	34.75			31.16	N/A	N/A	N/A	34.86	34.75		30.27	N/A	N/A	39.80	34.86	34.75		30.44	N/A	N/A	N/A	34.86	34.75		30.37	42.20	N/A	37.71	35.45	36.50	
13N	30.12	N/A	N/A	41.78	34.78	35.37			28.47	39.42	N/A	N/A	34.78	35.37		27.05	N/A	N/A	38.24	34.78	35.37		28.80	N/A	N/A	44.72	34.78	35.37		28.10	N/A	N/A	N/A	35.45	36.50	
14N	30.14	N/A	N/A	N/A	34.78	35.37			29.53	42.71	N/A	N/A	34.78	35.37		28.44	N/A	N/A	44.75	34.78	35.37		27.16	N/A	N/A	42.08	34.78	35.37		28.14	N/A	N/A	41.68	35.45	36.50	
15N	30.59	N/A	N/A	N/A	34.86	34.75			28.02	N/A	N/A	42.06	34.57	35.53		27.35	N/A	N/A	40.98	34.57	35.53		28.56	44.14	N/A	N/A	34.57	35.53		27.48	N/A	N/A	38.61	35.45	36.50	
16N	34.93	N/A	N/A	N/A	34.78	35.37			29.22	N/A	36.63	N/A	34.78	35.37		27.68	N/A	N/A	43.37	34.78	35.37		28.81	N/A	N/A	N/A	34.78	35.37		28.43	N/A	41.70	N/A	34.84	37.00	
17N	28.97	N/A	N/A	N/A	34.86	34.75			28.22	N/A	N/A	41.10	34.86	34.75		28.56	N/A	N/A	39.98	34.86	34.75		28.42	N/A	N/A	N/A	34.86	34.75		28.13	N/A	N/A	N/A	34.84	37.00	
18N	30.30	41.06	N/A	N/A	34.62	35.53			31.55	N/A	N/A	N/A	34.86	34.75		29.71	36.96	N/A	N/A	34.86	34.75		29.12	N/A	N/A	N/A	34.86	34.75		29.32	N/A	N/A	N/A	34.84	37.00	
19N	28.61	N/A	N/A	40.87	34.83	36.97			29.38	41.11	N/A	N/A	34.83	36.97		28.51	N/A	N/A	N/A	34.83	36.97		29.18	N/A	N/A	44.22	34.83	36.97		28.64	N/A	N/A	42.16	34.84	37.00	
20N	29.54	N/A	N/A	38.64	34.83	36.97			28.95	N/A	N/A	43.42	34.83	36.97		31.05	N/A	39.29	N/A	34.83	36.97		29.57	N/A	N/A	N/A	34.83	36.97		30.06	N/A	N/A	N/A	34.84	37.00	
1P	27.99	25.93	28.19	28.31	34.85	36.50			30.66	N/A	N/A	N/A	34.83	36.97		26.43	N/A	N/A	44.16	34.83	36.97		23.62	N/A	N/A	41.22	34.83	36.97		27.66	28.73	30.42	30.70	35.45	36.50	
2P	30.23	19.81	20.86	21.52	35.05	36.98			30.64	N/A	N/A	N/A	34.83	36.97		27.81	N/A	N/A	40.70	34.83	36.97		28.70	N/A	N/A	40.85	34.83	36.97		28.87	23.25	24.25	25.45	35.45	36.50	
3P	30.50	20.67	20.84	20.54	35.45	36.50			28.38	N/A	N/A	43.41	34.83	36.97		29.17	N/A	N/A	N/A	34.83	36.97		31.14	N/A	N/A	40.94	34.83	36.97		29.01	20.31	20.61	20.46	35.45	36.50	
4P	27.63	32.52	33.79	34.24	34.75	34.73			25.68	36.67	N/A	36.33	34.75	34.73		27.20	36.60	44.43	44.24	34.75	34.73		27.27	44.23	N/A	41.82	34.75	34.73		27.08	33.09	34.22	34.70	35.82	34.13	
5P	28.43	15.32	16.49	16.58	34.82	38.17			26.46	41.00	41.41	40.55	34.82	38.17		29.24	N/A	N/A	N/A	34.82	38.17		27.30	42.96	44.99	41.84	34.82	38.17		28.82	18.01	18.74	18.38	35.82	34.13	
6P	29.03	26.65	28.78	29.38	34.82	38.17			27.17	36.47	36.01	42.53	34.82	38.17		27.35	N/A	N/A	38.54	34.82	38.17		29.59	N/A	N/A	41.82	34.82	38.17		28.07	29.18	30.90	31.17	35.82	34.13	
7P	29.10	21.48	23.29	23.16	35.36	37.96			29.99	N/A	N/A	N/A	35.36	37.96		28.23	42.18	N/A	N/A	35.36	37.96		27.83	N/A	42.17	37.90	35.36	37.96		29.04	23.68	25.06	24.96	35.82	34.13	
8P	29.60	32.91	33.68	33.48	35.36	37.96			29.50	N/A	N/A	39.25	35.36	37.96		28.65	35.15	37.22	44.27	35.36	37.96		29.08	N/A	N/A	42.11	35.36	37.96		28.73	33.72	34.38	34.91	35.82	34.13	
9P	28.41	21.68	22.80	22.99	35.36	37.96			28.99	N/A	N/A	37.58	35.36	37.96		28.80	N/A	N/A	37.14	35.36	37.96		30.19	N/A	N/A	43.22	35.36	37.96		28.09	23.05	24.41	24.19	34.22	34.24	
10P	28.27	20.07	21.38	21.71	35.14	38.32			29.83	N/A	N/A	N/A	35.14	38.32		28.76	N/A	N/A	N/A	35.14	38.32		28.11	36.28	36.04	37.87	35.14	38.32		30.80	25.15	26.27	26.49	35.14	37.18	
11P	29.45	21.49	23.53	24.17	35.49	38.34			27.67	43.23	N/A	N/A	35.49	38.34		28.29	N/A	N/A	N/A	35.49	38.34		29.39	37.08	N/A	N/A	35.49	38.34		30.11	24.67	26.74	27.12	35.14	37.18	
12P	28.25	17.45	19.10	19.55	35.36	37.96			32.04	N/A	N/A	N/A	35.36	37.96		27.98	N/A	N/A	40.87	35.36	37.96		28.57	N/A	N/A	42.20	35.36	37.96		31.54	21.92	23.31	23.86	35.14	37.18	
13P	28.56	20.85	21.81	21.73	34.72	37.90			28.70	37.18	N/A	N/A	34.72	37.90		27.68	37.09	N/A	38.44	34.72	37.90		28.85	N/A	N/A	N/A	34.72	37.90		29.62	24.14	24.72	24.63	35.14	37.18	
14P	29.29	17.10	19.07	19.20	34.72	37.90			29.42	N/A	N/A	N/A	33.76	38.43		28.22	N/A	N/A	41.53	33.76	38.43		26.30	N/A	N/A	N/A	33.76	38.43		28.85	19.40	20.95	21.14	35.14	37.18	
15P	28.49	23.06	24.23	24.17	34.72	37.90			27.28	38.62	N/A	37.70	34.89	37.21		28.20	44.63	37.09	36.69	34.89	37.21		28.32	41.72	N/A	42.70	34.89	37.21		30.08	26.01	27.06	27.09	35.14	37.18	
16P	28.01	21.08	22.30	22.20	34.72	37.90			27.91	43.50	N/A	44.66	34.72	37.90		27.89	N/A	N/A	42.15	34.72	37.90		28.25	35.86	36.22	36.62	34.72	37.90		29.42	23.36	24.73	24.56	35.14	37.18	
17P	27.86	22.61	24.66	24.47	34.72	37.90			27.56	N/A	42.57	41.58	34.72	37.90		28.17	N/A	N/A	39.26	34.72	37.90		27.19	N/A	N/A	N/A	34.72	37.90		29.61	28.27	30.14	30.08	35.14	37.18	
18P	27.79	31.22	31.20	30.91	34.72	37.90			29.22	N/A	36.63	N/A	34.72	37.90		27.68	N/A	N/A	43.37	34.72	37.90		28.81	N/A	N/A	N/A	34.72	37.90		28.34	32.06	32.87	32.60	34.84	37.00	
19P	27.81	33.73	32.82	33.39	33.76	38.43			28.22	N/A	N/A	41.10	33.76	38.43																						

Positives

A	B	C	D	E	F	G	H	I	J	K	L	M
	Ct _{RPP}			Ct _{N2}			Ct _{E1}			Ct _{S6}		
Pool name	Individual	Pool	Ct difference	Individual	Pool	Ct difference	Individual	Pool	Ct difference	Individual	Pool	Ct difference
1P	27.99	27.66	-0.33	25.93	28.73	2.80	28.19	30.42	2.23	28.31	30.70	2.39
2P	30.23	28.87	-1.36	19.81	23.25	3.43	20.86	24.25	3.39	21.52	25.45	3.93
3P	30.50	29.01	-1.50	20.67	20.31	-0.36	20.84	20.61	-0.22	20.54	20.46	-0.08
4P	27.63	27.08	-0.55	32.52	33.09	0.57	33.79	34.22	0.43	34.24	34.70	0.45
5P	28.43	28.82	0.39	15.32	18.01	2.69	16.49	18.74	2.25	16.58	18.38	1.79
6P	29.03	28.07	-0.95	26.65	29.18	2.52	28.78	30.90	2.12	29.38	31.17	1.79
7P	29.10	29.04	-0.05	21.48	23.68	2.20	23.29	25.06	1.77	23.16	24.96	1.80
8P	29.60	28.73	-0.88	32.91	33.72	0.81	33.68	34.38	0.70	33.48	34.91	1.43
9P	28.41	28.09	-0.31	21.68	23.05	1.37	22.80	24.41	1.61	22.99	24.19	1.20
10P	28.27	30.80	2.53	20.07	25.15	5.08	21.38	26.27	4.89	21.71	26.49	4.78
11P	29.45	30.11	0.66	21.49	24.67	3.17	23.53	26.74	3.21	24.17	27.12	2.95
12P	28.25	31.54	3.28	17.45	21.92	4.48	19.10	23.31	4.21	19.55	23.86	4.31
13P	28.56	29.62	1.06	20.85	24.14	3.29	21.81	24.72	2.90	21.73	24.63	2.90
14P	29.29	28.85	-0.44	17.10	19.40	2.31	19.07	20.95	1.88	19.20	21.14	1.95
15P	28.49	30.08	1.59	23.06	26.01	2.95	24.23	27.06	2.83	24.17	27.09	2.92
16P	28.01	29.42	1.41	21.08	23.36	2.28	22.30	24.73	2.43	22.20	24.56	2.35
17P	27.86	29.61	1.75	22.61	28.27	5.66	24.66	30.14	5.48	24.47	30.08	5.61
18P	27.79	28.34	0.54	31.22	32.06	0.84	31.20	32.87	1.67	30.91	32.60	1.70
19P	27.81	28.20	0.39	33.73	35.50	1.78	32.82	35.10	2.28	33.39	36.11	2.72
20P	28.46	28.60	0.13	21.16	22.62	1.46	22.26	24.04	1.78	22.16	24.09	1.93
21P	27.06	28.06	1.00	33.26	35.91	2.65	33.12	35.93	2.81	32.61	34.74	2.13

Regression

Pool name	Ct _N		Ct _E		Ct _S	
	Individual	Pool	Individual	Pool	Individual	Pool
1P	25.93	28.73	28.19	30.42	28.31	30.70
2P	19.81	23.25	20.86	24.25	21.52	25.45
3P	20.67	20.31	20.84	20.61	20.54	20.46
4P	32.52	33.09	33.79	34.22	34.24	34.70
5P	15.32	18.01	16.49	18.74	16.58	18.38
6P	26.65	29.18	28.78	30.90	29.38	31.17
7P	21.48	23.68	23.29	25.06	23.16	24.96
8P	32.91	33.72	33.68	34.38	33.48	34.91
9P	21.68	23.05	22.80	24.41	22.99	24.19
10P	20.07	25.15	21.38	26.27	21.71	26.49
11P	21.49	24.67	23.53	26.74	24.17	27.12
12P	17.45	21.92	19.10	23.31	19.55	23.86
13P	20.85	24.14	21.81	24.72	21.73	24.63
14P	17.10	19.40	19.07	20.95	19.20	21.14
15P	23.06	26.01	24.23	27.06	24.17	27.09
16P	21.08	23.36	22.30	24.73	22.20	24.56
17P	22.61	28.27	24.66	30.14	24.47	30.08
18P	31.22	32.06	31.20	32.87	30.91	32.60
19P	33.73	35.50	32.82	35.10	33.39	36.11
20P	21.16	22.62	22.26	24.04	22.16	24.09
21P	33.26	35.91	33.12	35.93	32.61	34.74

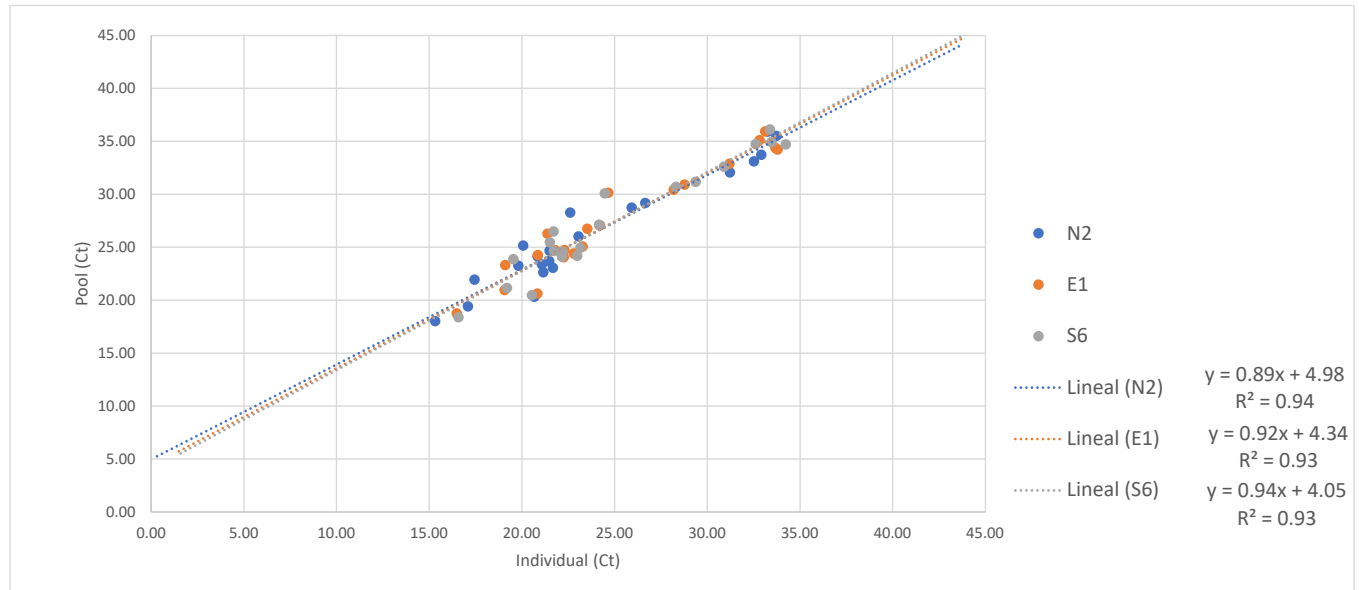

Gene	Pool			Individual		
	LOD	95% CI lower	95% CI upper	LOD	95% CI lower	95% CI upper
N	37.29	36.91	37.67	36.30	35.88	36.73
E	37.29	36.91	37.67	35.82	35.40	36.23
S	37.29	36.91	37.67	35.36	34.96	35.77

For a pool which is at the limit of detection, the individual sample would have had a Ct around 36.30 for N2. This means that during the pooling procedure samples with Cts between 36.30 and 37.29 would have been detected using individual testing but will not be due to pooling.