

Supplementary Material


Table of content

- (A) **Table 1: Study Team** 2
- (B) **Figure 1: Study Flow** 3
- (C) **Table 2: Detailed list of symptoms for all PCR positive participants**..... 4
- (D) **Table 3: Sensitivity and Specificity overall and by subgroups**..... 6
- (E) **Table 4: Ag-RDT – RT-PCR discrepant analysis: Buffer solution RT-PCR-results of Ag-RDT false-positive and Ag-RDT false-negative retained samples** 7

(A) Table 1: Study Team

Public Health Authority, Rhein-Neckar-Region, Heidelberg, Germany	Dr. K. Assaad,
	Dr. A. Fuhs
	Dr. C. Harter
	C. Schulze
	G. Schmitt
Division of Clinical Tropical Medicine, Heidelberg University Hospital, Heidelberg Germany	Loai Abutaima
	Rico Müller
	Martina Fink
	Mathilde Fougereau
	Maximilian Schirmer
	Annika Small
	Matthias Meinschmidt
	Valerie Dürr
	Alina Schuckert
	Ann-Kathrin Backes
	Salome Steinke
	Henrik Ellinghaus
	Magdalena Mikula
	Nele Schäfer

(B) Figure 1: Study Flow

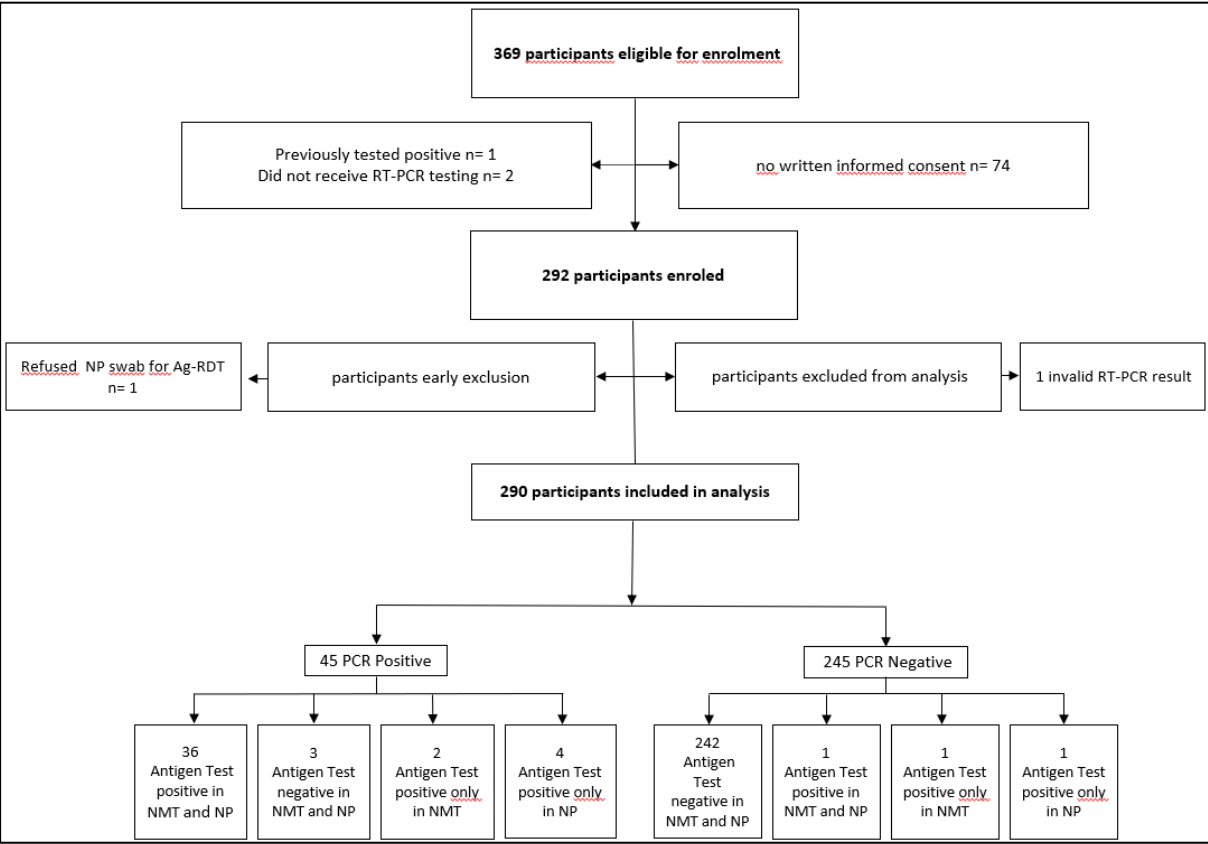

(C) Table 2: Detailed list of symptoms for all PCR positive participants

CT value: E-Gene	Viral load (log ₁₀ RNA copies/mL)	Result Ag-RDT NMT swab	Result Ag-RDT NP swab	Increased temperature/fever	Cough	Productive Cough	Sore throat	Dyspnoea	Body aches/muscle pain	Fatigue	Headache	Runny nose	Chest pain	Diarrhea	Nausea / Vomitus	Loss of taste/ smell	Other symptoms
13.1	9.9	positive	positive	No	Yes	No	No	No	Yes	Yes	Yes	No	No	No	No	No	Yes
25.7	6.2	positive	positive	No	Yes	No	No	No	Yes	Yes	Yes	No	No	Yes	No	No	No
22.6	7.1	positive	positive	Yes	Yes	No	Yes	No	Yes	Yes	Yes	No	Yes	No	No	Yes	No
31.2	4.5	positive	negative	No	No	No	Yes	No	Yes	Yes	Yes	No	No	No	No	No	No
26.0	6.1	positive	positive	No	No	No	No	No	No	No	Yes	Yes	No	No	No	Yes	No
22.1	7.2	negative	positive	Yes	Yes	No	Yes	No	Yes	Yes	Yes	No	No	Yes	Yes	No	
23.1	6.9	positive	positive														
26.7	5.9	positive	positive	No	No	No	No	No	No	No	No	No	No	No	No	Yes	No
16.1	9.0	positive	positive	No	Yes	Yes	Yes	No	Yes	Yes	No	Yes	No	No	No	No	No
16.5	8.9	positive	positive	Yes	Yes	No	Yes		No	Yes	Yes	No	No	No	No	No	No
19.7	7.9	positive	positive	No	No	No	Yes	No	No	Yes	Yes	No	No	No	No	No	No
26.7	5.9	negative	negative	No	No	No	No	No	No	No	Yes	No	No	No	No	No	No
16.6	8.9	positive	positive	Yes	No	No	No	No	No	No	Yes	No	No	No	No		No
18.9	8.2	positive	negative	No	No	No	No	No	No	No	No	Yes	No	No	No	No	Yes
23.8	6.7	positive	positive	No	No	No	No	No	Yes	Yes	No	Yes		No	No	Yes	No
16.7	8.8	positive	positive	No	Yes	No	Yes	No	Yes	Yes	Yes	No	Yes	No	No	No	No
17.8	8.5	positive	positive	Yes	No	No	No	No	Yes	No	No	No	No	No	No	No	No
20.1	7.8	positive	positive														
16.4	8.9	positive	positive	No	Yes		Yes	No	No	Yes	Yes	No	No	No	No	No	No
30.6	4.7	negative	negative														
17.9	8.5	positive	positive	Yes	No	No	No	No	Yes	Yes	Yes	No	No	No	No	No	No
21.2	7.5	positive	positive	Yes	No	Yes	Yes	No	Yes	Yes	Yes	No	Yes	No	No	No	Yes
18.8	8.2	positive	positive	Yes	No	No	Yes	No	Yes	Yes	Yes	Yes	No	No	No	No	No
27.7	5.6	positive	positive	Yes	Yes	Yes	No	No	Yes	Yes	Yes	No	No	No	No	Yes	No
12.7	10.0	positive	positive	No	Yes	Yes	No	No	No	Yes	Yes	Yes	No	No	No	No	No
16.5	8.9	positive	positive	No	Yes	Yes	No	No	Yes	No	Yes	Yes	No	Yes	No	No	No
33.8	3.8	negative	positive														
22.5	7.1	positive	positive	No	No	No	No	No	Yes	No	Yes	No	No	No	No	Yes	No

CT value: E-Gene	Viral load (log ₁₀ RNA copies/mL)	Result Ag-RDT NMT swab	Result Ag-RDT NP swab	Increased temperature/fever	Cough	Productive Cough	Sore throat	Dyspnoe	Body aches/muscle pain	Fatigue	Headache	Runny nose	Chest pain	Diarrhea	Nausea / Vomitus	Loss of taste/ smell	Other symptoms
12.9	9.9	positive	positive	Yes	Yes	Yes	Yes	No	No	Yes	No	Yes	No	No	No	No	No
25.9	6.1	positive	positive	Yes	Yes	Yes	No	No	Yes	Yes	Yes	Yes	No	No	No	No	No
18.8	8.2	positive	positive	Yes	No	No	No	No	Yes	Yes	Yes	No	No	No	No	No	Yes
23.6	6.8	positive	positive		Yes	No	Yes	No	Yes	Yes	Yes	Yes	No	No	No	No	Yes
34.5	3.6	negative	negative	No	Yes	No	No	No	No	No	No	Yes	No	No	No	No	No
19.9	7.9	positive	positive	No	Yes	No	Yes	No	No	Yes	Yes	No	No	Yes	No	Yes	No
23.1	6.9	positive	positive	No	Yes	Yes	Yes	No	Yes	Yes	Yes	Yes	No	No	Yes	No	No
31.2	4.5	positive	positive	No	No	No	No	No	No	Yes	Yes	Yes	No	Yes	No	Yes	No
21.4	7.4	positive	positive														
29.7	5.0	negative	positive														
22.8	7.0	positive	positive	No	Yes	No	No	No	Yes	Yes	Yes	No	Yes	No	No	No	Yes
22.5	7.1	positive	positive	Yes	Yes	Yes	No	Yes	No	Yes	Yes	No	No	No	No	No	No
19.9	7.9	positive	positive														
26.3	6.0	positive	positive														
32.7	4.1	negative	positive	Yes	Yes	No	Yes	Yes	Yes	Yes	Yes	Yes	Yes	No	No	Yes	No
20.2	7.8	positive	positive	Yes	Yes	No	No	No	Yes	Yes	Yes	Yes	No	No	No	No	Yes
19.5	8.0	positive	positive	No	Yes	No	No	No	Yes	No	Yes	Yes	No	No	No	No	No

(D) Table 3: Sensitivity and Specificity overall and by subgroups

	Sampling technique	Sensitivity (%; 95% CI)	Specificity (%; 95% CI)	Positive Percent Agreement	Negative Percent Agreement
Overall	NP	40* / 45 (88.9%; 76.5% - 95.5%)	243 / 245 (99.2%; 97.1% - 99.8%)	37* / 42** (88.1%; 75.0% - 94.8%)	245 / 248 (98.8%; 96.5% - 99.6%)
	NMT	38 / 45 (84.4%; 71.2% - 92.3%)	243 / 245 (99.2%; 97.1% - 99.8%)		
Viral load ≥7 log₁₀ SARS-CoV-2 RNA copies/ml	NP	26 / 27 (96.3%; 81.7% - 99.8%)	n.a.	25 / 26 (96.2%; 81.1% - 99.8%)	n.a.
	NMT	26 / 27 (96.3%; 81.7% - 99.8%)	n.a.		
Viral load <7 log₁₀ SARS-CoV-2 RNA copies/ml	NP	14 / 18 (77.8%; 54.8% - 90.1%)	n.a.	11 / 14 (78.6%; 52.4% - 92.4%)	n.a.
	NMT	12 / 18 (66.7%; 43.7% - 83.7%)	n.a.		
symptomatic	NP	33/37 (89.2%, 75.3% - 95.7%)	94/96 (97.9%, 81.4% - 99.4%)	33 / 35 (91.4%, 77.6% - 97.0%)	96 / 98 (98.0%, 92.8% - 99.4%)
	NMT	33/37 (89.2%, 75.3% - 95.7%)	95/96 (99.0%, 94.3% - 99.9%)		
asymptomatic	NP	7/8 (87.5%, 52.9% - 99.4%)	147/147 (100%, 97.5 - 100%)	5 / 7 (71.4%, 35.9% - 91.8%)	147 / 148 (99.3%, 96.3% - 100%)
	NMT	5/8 (62.5%, 30.6% - 86.3%)	146/147 (99.3%, 96.2% - 100%)		

Abbreviations: n.a.: not applicable; NP: nasopharyngeal; NMT: nasal mid-turbinate; CI: confidence interval

**including one false-positive in NMT and NP

**including two false-positive in NP

(E) Table 4: Ag-RDT – RT-PCR discrepant analysis: Buffer solution RT-PCR-results of Ag-RDT false-positive and Ag-RDT false-negative retained samples

Ag-RDT false-positives									
Ag-RDT NMT swab	Ag-RDT NP swab	RT-PCR	Assay	RT-PCR buffer NMT sample	RT-PCR buffer NP sample	Sampling comment	Probe aspect	Symptom duration (days)	
positive	negative	negative	TibMolBiol	negative	negative	none	NMT: mucous NP: clear	asymptomatic	
positive	positive	negative	TibMolBiol	positive (Ct 27.3; VL* 6.3)	positive (Ct 31.8; VL* 5.0)	none	NMT: clear NP: mucous	3	
negative	positive	negative	TibMolBiol	negative	negative	none	NMT: clear NP: mucous	6	
Ag-RDT false-negatives									
Ag-RDT NMT swab	Ag-RDT NP swab	Ct-value	Viral load*	Assay	RT-PCR buffer NMT sample	RT-PCR buffer NP sample	Sampling comment	Probe aspect	Symptom duration (days)
negative	positive	22.1	7.2	TibMolBiol	sample got lost	not tested	none	NMT: clear NP:clear	1
negative	positive	29.7	5.0	TibMolBiol	negative	not tested	none	NMT: mucous NP:clear	asymptomatic
negative	positive	32.7	4.1	TibMolBiol	positive (Ct 33.7; VL* 4.4)	not tested	none	NMT: mucous NP: mucous,bloody spots	n.a.
negative	positive	33.8	3.8	TibMolBiol	negative	not tested	none	NMT: clear NP: mucous	asymptomatic
positive	negative	18.9	8.2	TibMolBiol	not tested	negative	none	NMT: clear NP:clear	1
positive	negative	31.2	4.5	TibMolBiol	not tested	sample got lost	none	NMT: clear NP:clear	1
Ct: cycle threshold; Ag-RDT: antigen-detecting rapid diagnostic test; NMT: nasal mid-turbinate; NP: nasopharyngeal. n.a.: not available; *log ₁₀ SARS-CoV-2 RNA copies/ml									