

## Supplementary Information

### Manuscript: SARS-CoV-2 wastewater surveillance in Germany: long-term PCR monitoring, suitability of primer/probe combinations and biomarker stability

Authors: Johannes Ho, Claudia Stange, Rabea Suhrborg, Christian Wurzbacher, Jörg E.

Drewes, Andreas Tiehm

	Infection value shift in days																					
$r^2$	0	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21
	0.44	0.49	0.56	0.60	0.63	0.67	0.71	0.75	0.77	0.80	0.81	0.83	0.85	0.86	0.87	0.88	0.89	0.88	0.87	0.85	0.84	0.83

Fig. S1. Correlation coefficients ( $r^2$ ) for infection numbers and biomarker concentrations with different time shifts from 0 to 21 days for the infection numbers. P values with Bonferroni-correction were below 0.001 for all correlations.

### Linear regression

Infection data not shifted (original data)

**Without intercept**

$$y = 6.65x$$

$$R^2 = 0.44$$

$$n = 89$$

$$p < 0.001$$

$$\text{LOQt: } 16.6 / 100,000$$

**With intercept**

$$y = 5.11x + 39.98$$

$$R^2 = 0.51$$

$$n = 89$$

$$p < 0.001$$

$$\text{LOQt: } 52.8 / 100,000$$

Infection data shifted by 16 days

**Without intercept**

$$y = 7.29x$$

$$R^2 = 0.89$$

$$n = 89$$

$$p < 0.001$$

$$\text{LOQt: } 18.2 / 100,000$$

**With intercept**



$$y = 6.74x + 9.21$$

$$R^2 = 0.91$$

$$n = 89$$

$$p < 0.001$$


$$\text{LOQt: } 26.1 / 100,000$$

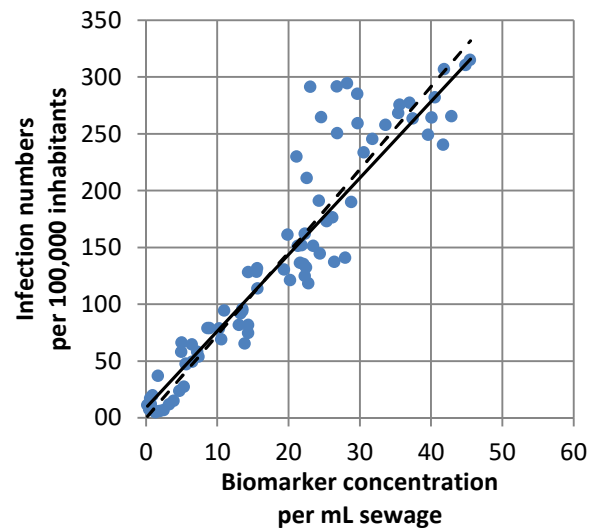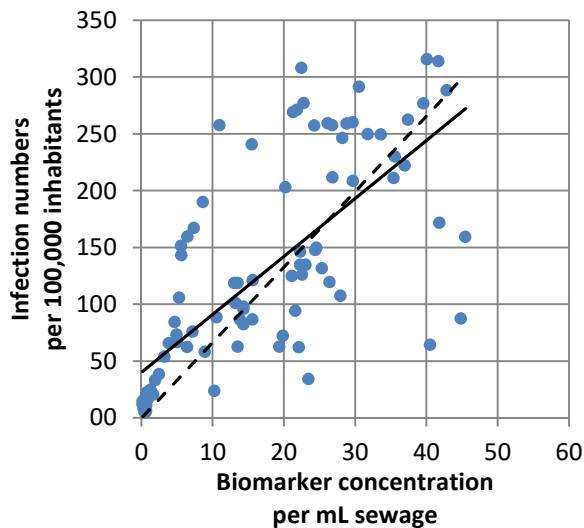


- - - trendline, intersection with 0,0

— trendline, w/o intersection

Fig. S2. Linear regression for infection data and ddPCR values (E and ORF gene as sliding average of three values). Left: original data, right: infection numbers were time-shifted by 16 days. Statistical analysis above each plot for each trend line with and without intercept. P values with Bonferroni-correction were below 0.001 for all correlations.

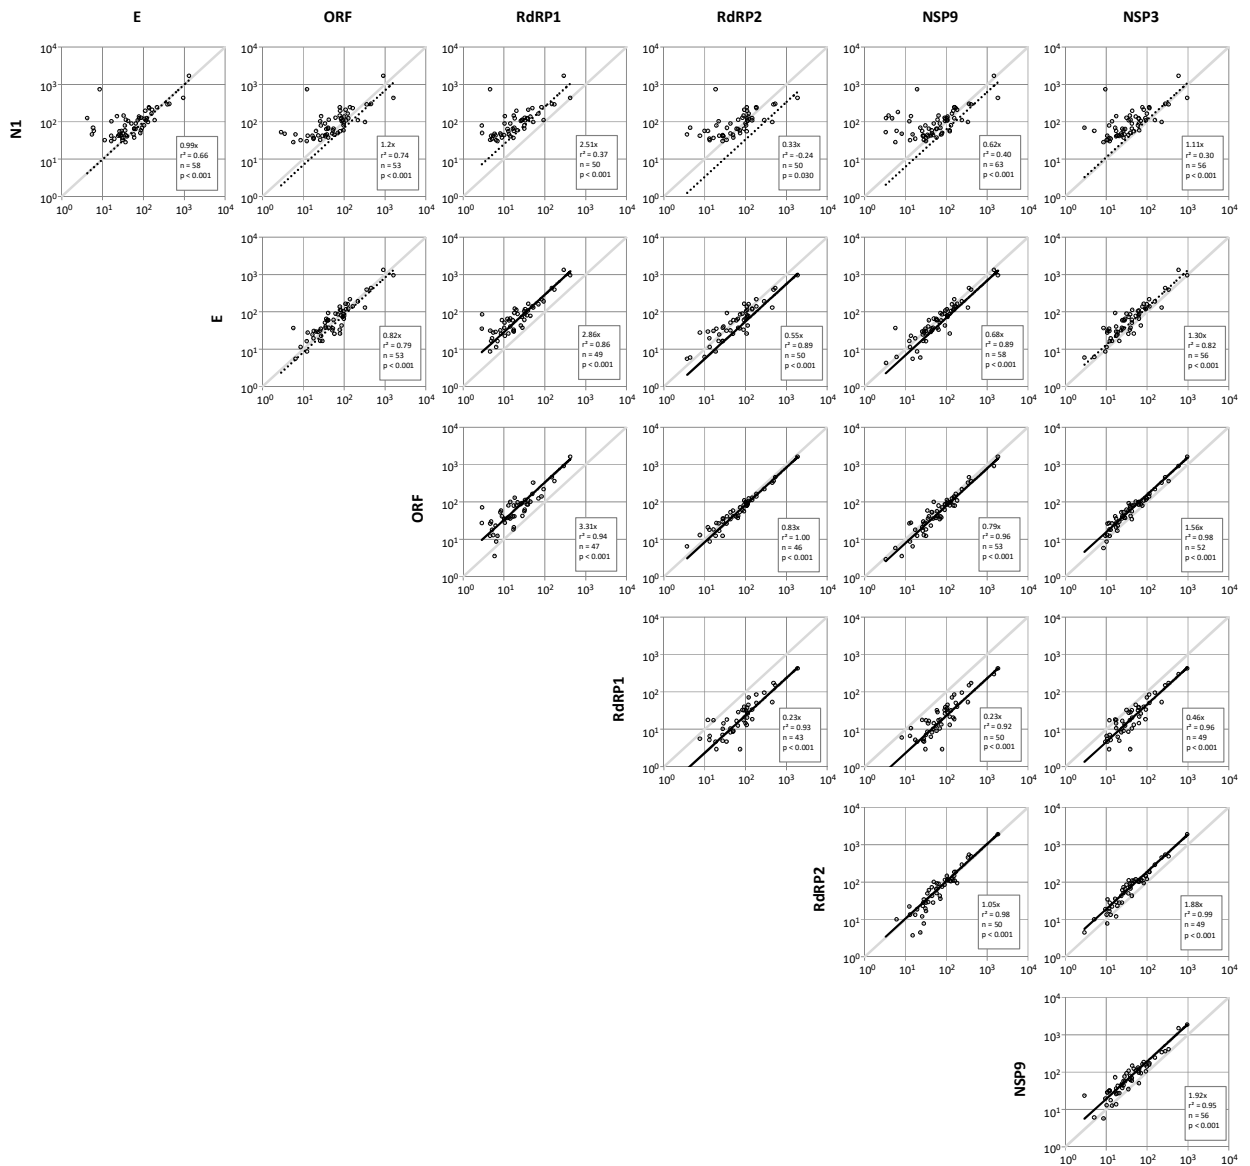

**Fig. S3.** Linear regressions of seven different primer/probe assays using a selection of 64 samples. Charts show gene copies per mL wastewater.

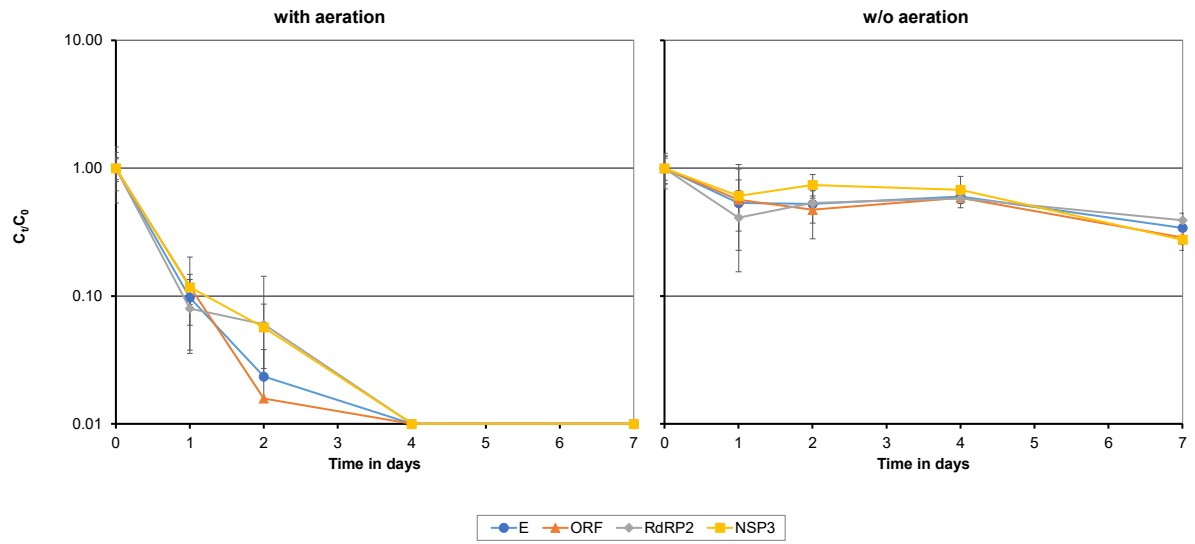

**Fig. S4.** Decay of SARS-CoV-2 specific targets over time in wastewater samples aerated with air (left) or nitrogen (right). Error bars represent standard deviations for the three independent test bottles (n = 3).