

Title Magnetocardiography for the diagnosis of coronary artery disease: a systematic review and meta-analysis

The authors

Their academic degrees, and affiliations are listed below:

1. Dr. Miao Yang[†], PhD, Department of Pediatric, Shengjing Hospital of China Medical University.
2. Mr. Chenxi Sun[†], PhD candidate, State Key Laboratory of Advanced Optical Communication Systems and Networks, School of Electronics, and Center for Quantum Information Technology, Peking University.
3. Mrs. Biying Zhao, PhD candidate, State Key Laboratory of Advanced Optical Communication Systems and Networks, School of Electronics, and Center for Quantum Information Technology, Peking University.
4. Mrs. Bo Wu, PhD candidate, Department of Pediatric, Shengjing Hospital of China Medical University.
5. Dr. Jing Xiang, PhD, Department of Neurology, The MEG Center, Cincinnati Children's Hospital Medical Center.
6. Dr. Man Xu, PhD, Department of Cardiology, Renmin Hospital of Wuhan University, Hubei Key Laboratory of Metabolic and Chronic Diseases, Wuhan.
7. Dr. Teng Wu, PhD, State Key Laboratory of Advanced Optical Communication Systems and Networks, School of Electronics, and Center for Quantum Information Technology, Peking University.

NOTE: This preprint reports new research that has not been certified by peer review and should not be used to guide clinical practice.

8. Dr. Jianwei Zhang, PhD, School of Physics, Peking University.

9. Dr. Wei Xu^{*}, PhD, Department of Pediatric, Shengjing Hospital of China Medical University.

10. Dr. Hong Guo, PhD, State Key Laboratory of Advanced Optical Communication Systems and Networks, School of Electronics, and Center for Quantum Information Technology, Peking University.

† These authors contributed equally to this work.

Corresponding author: * Wei Xu, xuw@sj-hospital.org, No.36 of Sanhao St., Heping District, Shenyang, Liaoning Province, 110004

The total word count of the manuscript: 5422

Abstract

Background: Globally, coronary heart disease (CHD) is a major public health issue because it significantly increases mortality and medical expenses. In the recent years, magnetocardiography (MCG) has shown its potential as a new tool for diagnosing CHD. However, the quantitative assessment of MCG currently used for CHD diagnosis are insufficient, preventing its full integration into routine clinical practice.

Methods: We searched PubMed (including MEDLINE), Embase, Web of Science, Cochrane Library, Scopus, China National Knowledge Infrastructure (CNKI), Wanfang Data, and ClinicalTrials.gov for studies published up to March 4, 2023. We systematically searched for studies that compare MCG (as the index test) with coronary angiography (as the standard reference) for diagnosing CHD in suspected population. Three authors assessed the quality of the included studies independently using the QUADAS-2 tool. We calculated the pooled value of the sensitivity and specificity of MCG using the bivariate model. To investigate clinical and methodological factors that might contribute to the statistical heterogeneity, we used meta-regression and subgroup analysis. This systematic review and meta-analysis has been conformed to PRISMA guidelines and registered with PROSPERO (number CRD42022332272).

Results: By searching, we found 174 studies, 18 of them included 2,571 subjects from 6 countries and regions and met the inclusion criteria. The combined values for sensitivity and specificity are 86% (95% CI: 80-91) and 79% (95% CI: 71-86), respectively. The summary receiver operating characteristic (SROC) curve's area under the curve was 0.90. We found significant statistical heterogeneity between studies (for

sensitivity, $I^2=94.22\%$ (95% CI: 92.48-95.96), $Q=294.11$, $P<0.01$; for specificity, $I^2=88.98\%$ (95% CI: 84.95-93.01), $Q=154.26$, $P<0.01$.

Conclusion: Given its high sensitivity, MCG has a high value for diagnosing CHD, especially in primary screening. Further investigation is required to examine additional factors that may affect the performance of MCG considering the limited clinical trials and sample size.

Key words: coronary heart disease, magnetocardiography, electrocardiography.

Non-standard Abbreviations and Acronyms.		
No.	Abbreviation	Full name
1	ACS	acute coronary syndromes
2	AF	atrial fibrillation
3	AFL	atrial flutter
4	AMI	acute myocardial infarction
5	AP	angina pectoris
6	AR	arrhythmias
7	AUC	the area under the curve
8	AVB	atrioventricular block
9	BBB	bundle branch block
10	CABG	coronary artery bypass surgery
11	CAG	coronary angiography
12	CBBB	complete bundle branch block
13	CDV	current density vector
14	CHD	coronary heart disease
15	CI	confidence interval
16	CK-MB	creatine kinase-MB isoenzyme
17	CM	cardiomyopathy
18	CNKI	China National Knowledge Infrastructure
19	CTCO	chronic total coronary occlusion

20	CVEI	complex ventricular excitation index
21	DCM	dilated cardiomyopathy
22	DM	diabetes mellitus
23	ECD	epicardial current density
24	ECG	electrocardiography
25	ECHO	echocardiography
26	ED	exertional dyspnea
27	EI	electrolyte imbalance
28	ESRF	end stage renal failure
29	FAPB	frequent atrial premature beats
30	FTW	flat T wave
31	HAP	hospital-admitted patient
32	HF	heart failure
33	HNOCM	hypertrophic nonobstructive cardiomyopathy
34	HOCM	hypertrophic obstructive cardiomyopathy
35	HTN	hypertension
36	HUP	hemodynamically unstable patient
37	IC	integral change
38	IHD	ischemic heart disease
39	ITW	inverted T wave
40	IVB	intraventricular block

41	LV	left ventricular
42	LVD	left ventricular dysfunction
43	LVEF	left ventricular ejection fraction
44	MA	malignant arrhythmias
45	MCG	magnetocardiography
46	MD	magnetic dipole
47	MFM	magnetic field map
48	MI	myocardial infarction
49	MP	metallic prosthesis
50	MPI	myocardial perfusion imaging
51	MT	malignant tumor
52	OPM	optically pumped magnetometer
53	PA	pre-peak repolarization angle
54	PAD	pre-peak repolarization angular deviation
55	PCI	percutaneous coronary intervention
56	PI	pacemaker implantation
57	PoA	post-peak repolarization angle
58	PoAD	post-peak repolarization angular deviation
59	PoT	post-peak repolarization trajectory
60	PPAC	pre-post angle change
61	PT	pre-peak repolarization trajectory

62	PTP	pre-test probability
63	ROC curve	receiver operating characteristic curve
63	SAP	stable angina pectoris
64	SHD	structural heart disease
65	SI-QTc	smooth index QTc
66	SQUID	superconducting quantum interference device
67	SR	sinus rhythm
68	SROC	summary receiver operating characteristic
69	STE	ST-segment elevation
70	UAP	unstable angina pectoris
71	VAP	variant angina pectoris
72	VD	valve disease
73	VH	ventricular hypertrophy
74	VHD	valvular heart disease
75	VPB	ventricular premature beats
76	yo.	years old

Introduction

Ischemic heart disease (IHD) is of high incidence and mortality rate worldwide, with an estimated 240 million cases globally in 2020.¹ As the leading cause of death across low-, middle-, and high-income countries,² IHD has a rising percentage of the relevant death continuously.³

Coronary heart disease (CHD), the primary cause of IHD, is brought on by the narrowing of coronary arteries and has resulted in a significant medical burden globally. Adults in the United States experienced over 20 million cases of CHD between 2017 and 2020, or about 7.1% of the population.¹ In Canada, the estimated average annual hospitalization costs for CHD patients are projected to reach 2.2 billion Canadian dollars, not to mention additional economic burdens from medication expenses and loss of productivity.⁴

In recent years, magnetocardiography (MCG) has emerged as a promising method for diagnosing cardiovascular diseases. The cardiac magnetic field generated by the electrical activity of the heart is extremely weak, with a magnitude of about 10^{-11} T. MCG can be accurately measured with a high signal-to-noise ratio using highly sensitive quantum magnetometers positioned above the chest. Since myocardial cells' electrical activity is what causes the heart to contract, MCG offers a clear reflection of that activity and enables the assessment of cardiac function. Compared to morphological methods such as coronary angiogram (CAG) and echocardiogram (ECHO), MCG identifies cardiac abnormalities before significant morphological changes become apparent, potentially indicating an earlier indication of the presence of

lesions. MCG has a higher sensitivity for currents produced by abnormal cardiac activities despite having similar waveforms and origins to electrocardiography (ECG).⁵ Aside from that, MCG might be more sensitive to the subtle signals associated with early-stage disease due to the homogenous magnetic permeability in various tissues. Multiple studies have also revealed the particular advantages of MCG in detecting CHD. MCG has been shown to identify patients without abnormality of resting ECG,⁶ and has exhibited superior diagnostic performance when compared with ECHO and biochemical parameters such as cardiac troponin.⁷ In addition, recent research has identified a range of potential diagnostic markers for CHD, including QT dispersion,⁸ QRS complex duration,⁹ ST segment-related parameters,¹⁰ and so on, which hold promise for further enhancing the diagnostic capabilities of MCG.

It is crucial to obtain an accurate assessment of MCG's diagnostic capacity for the future, especially when considering the availability of flexible, affordable MCG devices based on OPM greatly which increases the viability of its clinical application. Initial clinical trials have been carried out internationally to achieve this. However, a single trial's sample size is always constrained by the lengthy duration and the challenge of locating suitable samples. It is challenging to come to an unbiased conclusion about the applicability and diagnostic efficacy of MCG because the outcomes of clinical trials can vary significantly due to individual differences, especially when the sample size is insufficient. Additionally, the transition of MCG from a research tool to its clinical application is hampered by the dearth of clinical evidence brought on by these limitations.

Systematic review and meta-analysis are statistical methods that integrate comprehensive results from multiple studies, thereby increasing the sample size and enhancing the accuracy of conclusions. These methods overcome the limitations of individual MCG trials and can provide more reliable evidence for clinical decision-making. Due to the enhanced focus and studies on MCG, adequate clinical trials of MCG can be integrated together for accurate evaluation as well as further conclusions. At the same time, MCG exhibits variations across diverse demographic groups, such as those with different ages, genders, and disease severities.¹¹ The MCG itself also has different measurement modes and diagnostic indicators.¹² A detailed analysis is necessary to identify the specific populations and circumstances where MCG is most effective, and provide more tailored guidance for clinical decision-making.

Methods

Search strategy and selection criteria

We reported findings based on the PRISMA guidelines¹³ (details in supplementary materials), and a review protocol was registered in PROSPERO (CRD42022332272). For this systematic review and meta-analysis, we searched PubMed (including MEDLINE), Embase, Web of Science, Cochrane Library, Scopus, China National Knowledge Infrastructure (CNKI), Wanfang Data, and ClinicalTrials.gov for studies published up to March 4, 2023. We included all studies published in any language about patients with suspected CHD, which report the diagnostic results of MCG (as index test) and CAG (as reference standard) in all subjects. Studies based on immature machine

learning are excluded due to applicability concerns. Studies should be cross-sectional design. To be eligible, studies should recruit patients with suspected CHD symptoms, and all subjects should undergo both MCG and CAG, and we can obtain the value of the entries in the diagnostic 2×2 table through the information provided in the article (details in supplementary materials).

Data extraction

CS, BZ and MY independently screened the titles and abstracts of the articles obtained from the database searches to initially exclude studies against eligibility criteria. They then conducted a thorough examination of the full text of the remaining studies to determine whether they met the inclusion criteria. When dealing with studies containing duplicated data, our approach was to selectively include them based on the principle of avoiding data overlap and ensuring the broadest possible range of patient inclusion times. Any disagreements regarding the inclusion of a study were resolved by WX. Additionally, BZ and CS reviewed the reference lists of the searched studies for potentially relevant articles that were missed during the initial screening process. To ensure accuracy and completeness of the data, BZ and MY contacted relevant researchers to inquire about unpublished trials. BZ and MY extracted the data from eligible studies independently, and the results were verified by CS and WX.

We extracted the following data from the eligible articles: first author, year of publication, subjects, selected diagnostic criteria of CAG and MCG, diagnostic 2×2 table of MCG. If available, we also extracted the diagnostic 2×2 table of ECG. In case

where the results of multiple diagnostic indicators for MCG were reported, we extracted the results with the highest Youden Index for further analysis.

Quality assessment

BZ and MY independently assessed the quality of the included studies based on QUADAS-2 to evaluate the risk of bias and applicability from four aspects, including patient selection, index test, reference standard, and flow and timing. For cases of disagreement, consensus was achieved from CS. The quality assessment data were stored in Microsoft Excel® LTSC MSO (16.0.14332.20540).

Data analysis

We used the 2×2 table to evaluate the diagnostic performance of MCG (table S11). With STATAMP 18, we employed the bivariate model to the sensitivity and specificity with their corresponding 95% confidence intervals (CI) for each study and the pooled data. Furthermore, we generated a SROC curve to obtain a quantitative evaluation of the diagnostic value of MCG by calculating the area under the SROC curve (AUC).

We utilized Higgins and Thompson's I^2 and Cochran's Q to quantitatively assess the degree of statistical heterogeneity among studies. For the meta-regression and subgroup analysis, we explore three potential variables that may result in significant heterogeneity, including the presence of stress tests, the threshold of the gold standard, and the patient's resting ECG status. The stress test group comprises studies that measured during exercise, recovery from exercise, or after administration of

dobutamine, while the resting group only includes studies that measured the MCG of the subjects at rest. The mild group includes studies using a threshold of 50% for CAG, which means that patients with >50% stenosis are diagnosed as CHD, while the severe group use a threshold of 70%. The silent group includes studies that screened suspected CHD patients with normal resting ECG, while the ensemble group included all patients with suspected CHD.

Role of the funding source

The study design, data collection, data analysis, data interpretation, and manuscript writing were performed without any involvement from the funders. The corresponding author had complete access to all the data in the study and were responsible for the decision to submit for publication.

Results

From database searches, we found 130 studies. From international trial registries search, we found 44 relevant articles. After removing duplicates and after initial screening, that number dropped to 30. 18 studies were chosen for the meta-analysis after reading the full texts (figure 1). Studies were excluded from this process mainly due to the irrelevant content and various experimental techniques (table S12, table S13).

The 18 eligible studies were published between 2003 and 2023 and included a total of 2,571 participants from 6 different countries and regions: United States,^{14,15} China,¹⁶⁻²² Chinese Taiwan,^{23,24} Germany,^{7,25-29} Japan,³⁰ and Ukraine²⁷ (table 1). 4 studies

exclusively recruited suspected CHD patients with normal rest ECG, while the remaining 14 studies included suspected CHD patients regardless of their rest ECG status. 7 studies used a threshold of 50% for diagnosing CHD by CAG, while 10 studies used a threshold of 70%. 4 studies measured stress MCG, with 1 study performing measurements after the administration of dobutamine and 3 studies measuring MCG during or after exercise. 14 studies only measured the rest MCG.

The result of quality evaluation is shown in table 2 (details in supplementary materials). Due to the lack of recognized indices and the corresponding reference value, many studies choose to draw SROC curve to decide the best cut-off value, leading to high level of risk of bias in the index test. The results of each study and their combination are shown in the forest plot (figure 2). The pooled sensitivity of MCG for diagnosing CHD is 0.86 (95% CI: 0.80-0.91), and the pooled specificity is 0.79 (95% CI: 0.71-0.86). The area under SROC curve is 0.90 (95% CI: 0.87-0.92) (figure 3). The sensitivity analysis indicates the absence of significant publication bias (figure S1).

There is significant statistical heterogeneity between studies ($P<0.01$). The value of Cochran's Q for sensitivity and specificity are 294.11 and 154.26, respectively. The I^2 for sensitivity and specificity are 94.22% (95% CI: 92.48-95.96) and 88.98% (95% CI: 84.95-93.01), respectively. In the meta-regression and subgroup analysis, the value of sensitivity for mild CHD and severe CHD are 0.89 and 0.86, respectively, showing significant difference within subgroups ($P=0.01$). Other results of the analysis (table 3) are not significant due to the limited sample size.

Conclusions

This article presents a systematic review and meta-analysis aimed at evaluating the performance of MCG for diagnosing CHD. The study identified 18 eligible studies, which included 2,571 subjects from 6 countries and regions. The pooled sensitivity and specificity values for MCG are 86% (95% CI: 80-91) and 79% (95% CI: 71-86), respectively, indicating that MCG is of suitable for diagnosing CHD, especially in large-scale screening. The area under the SROC curve is 0.90, implying high diagnostic value of MCG.

This article provides a comprehensive evaluation of the diagnostic performance of MCG for diagnosing CHD using high-quality clinical trials. In contrast to the study of Rajender Agarwal *et al.*³¹ which reported analogous values for pooled sensitivity and specificity, our research employs a more comprehensive information retrieval process and conducts subgroup analysis. These analysis aim to provide deeper insights into the characteristics of MCG. According to our findings, MCG has a higher sensitivity for early CHD, which increases its benefits in CHD screening. Other analyses don't reveal any significant variations. We blame the small sample sizes in each subgroup for the issue. For instance, even though the silent group only consisted of 441 samples from 4 studies in the analysis of the patient's resting ECG status, the p-value of 0.09 is very close to the significant level and suggests potential findings for further investigation. Future investigation of additional factors that might have an impact on MCG performance will require more research.

More opportunities for conducting large population clinical trials across the globe are

made possible by the development of OPM-based MCG. However, given the lack of standardization in MCG procedures, it is crucial to optimize the design of future trials based on previous studies. The quality assessment shows unsatisfactory results concerning the risk of bias, mainly due to the unclear procedure followed in the trials. Firstly, patient selection should encompass suspected patients with varying severity levels, especially those who are challenging to diagnose accurately. Secondly, blind designs should be implemented for both CAG and MCG to minimize potential bias. Besides, to ensure reasonable flow and timing, an appropriate interval between MCG and CAG should be established. Considering the invasive nature of CAG and its potential impact on cardiac condition, MCG, as a noninvasive and quick examination, should be conducted within a 24-hour window before CAG to ensure comparable states of patients between the two tests. Additionally, in light of the absence of standardized diagnostic indices and their reference values for MCG, the existence of receiver operating characteristic (ROC) curves becomes essential to obtain sufficient values of thresholds. Large-scale global trials can be conducted based on the thresholds obtained during sufficient small-scale pre-experiment, thereby avoiding the bias introduced by the post-specified threshold.

Panel: Research in context

Evidence before this study

The rising global burden of coronary heart disease, with over 20 million cases in the United States in 3 years and nearly 2.2 billion Canadian dollars annual hospitalization

costs in Canada, underscores the urgent need for effective diagnostic methods. However, the lack of shielding methods with both high accuracy and low threshold poses a challenge. Magnetocardiography is a promising diagnostic tool that aligns with these requirements, and the recent development of unshielded OPM-based MCG devices further enhances its applicability. While many clinical trials have been conducted to obtain an accurate evaluation of MCG's diagnostic performance, their limited sample size impacts the accuracy of the results. To solve this problem, a comprehensive evaluation through systematic review and meta-analysis is crucial to gain deeper insights into MCG's diagnostic efficacy and drive evidence-based conclusions for its clinical application.

Added value of this study

Our systematic review and meta-analysis show that MCG is of high diagnostic value for CHD, with a value of 86% (95% CI: 80-91) and 79% (95% CI: 71-86) for pooled sensitivity and specificity, respectively. Compared with ECG, MCG significantly enhances diagnostic accuracy while maintaining comparable specificity. Furthermore, the subgroup analysis reveals that MCG exhibits higher sensitivity for early CHD, making it particularly suitable for large-scale screening.

Implications of all the available evidence

As MCG continues to evolve, an increase in relevant clinical trials is anticipated. Future trials should adopt a standardized design, encompass diverse patient selection,

incorporate blind designs, and establish reasonable MCG-CAG intervals. Utilizing ROC curves can aid in determining diagnostic indices' reference values for large-scale application. Additionally, integrating carbon electrodes into the MCG system may offer valuable insights for its clinical use across diverse demographics.

Contributors

MY contributed to conceptualization, data accessed and verified, data analysis, data interpretation, writing—original draft, and writing—review and editing. CS contributed to conceptualization, literature search, data accessed and verified, writing—original draft, and writing—review and editing. BZ, BW, JX, MX, JZ, and TW contributed to data interpretation, and writing—review and editing. WX contributed to data interpretation, supervision, and writing—review and editing, and decision to submit. HG contributed to project administration, supervision, and writing—review and editing, and decision to submit.

Data sharing

Extracted data and the Stata code in this study are fully reported in the supplementary material (pp. 14-16). Additional information will be available from the corresponding author upon reasonable request.

Acknowledgements

We thank F. Li from Guanghua School of Management, Peking University for the

manipulation in data analysis.

Sources of Funding

National Natural Science Foundation of China, National Key Research and Development Program of China, Basic scientific research project of Department of Education of Liaoning Province (LJKMZ20221186), Shenyang Public Health R&D Project (22-321-33-14), 345 Talent Project .

Disclosures

We declare no competing interests.

Reference

1. Tsao CW, Aday AW, Almarzooq ZI, Anderson CAM, Arora P, Avery CL, et al. Heart disease and stroke statistics-2023 update: a report from the American Heart Association. *Circulation* 2023; **147**: e93-621.
2. Lopez AD, Mathers CD, Ezzati M, Jamison DT, and Murray CJ. Global and regional burden of disease and risk factors, 2001: systematic analysis of population health data. *Lancet* 2006; **367**: 1747-57.
3. Lozano R, Naghavi M, Foreman K, Lim S, Shibuya K, Aboyans V, et al. Global and regional mortality from 235 causes of death for 20 age groups in 1990 and 2010: a systematic analysis for the Global Burden of Disease Study 2010. *Lancet* 2012; **380**: 2095-128.
4. Smolderen KG, Bell A, Lei Y, Cohen EA, Steg PG, Bhatt DL, et al. One-year costs associated with cardiovascular disease in Canada: insights from the REduction of Atherothrombosis for Continued Health (REACH) registry. *Can J Cardiol* 2010; **26**: e297-305.
5. Mäntynen V, Konttila T, and Stenroos M. Investigations of sensitivity and resolution of ECG and MCG in a realistically shaped thorax model. *Phys Med Biol* 2014; **59**: 7141.
6. Savard P, Cohen D, Lepschkin E, Cuffin BN, and Madias JE. Magnetic measurement of ST and TQ segment shifts in humans. Part I: Early repolarization and left bundle branch block. *Circ Res* 1983; **53**: 264-73.
7. Park JW, Hill PM, Chung N, Hugenholtz PG, and Jung F. Magnetocardiography predicts coronary artery disease in patients with acute chest pain. *Ann Noninvasive*

Electrocardiol 2005; **10**: 312-23.

8. Hailer B, Van Leeuwen P, Lange S, Pilath M, and Wehr M. Coronary artery disease may alter the spatial dispersion of the QT interval at rest. *Ann Noninvasive Electrocardiol* 1999; **4**: 267-73.

9. Korhonen P, Husa T, Tierala I, Väänänen H, Mäkijärvi M, Katila T, et al. QRS duration in high-resolution methods and standard ECG in risk assessment after first and recurrent myocardial infarctions. *PACE-Pacing Clin Electrophysiol* 2006; **29**: 830-36.

10. Kandori A, Kanzaki H, Miyatake K, Hashimoto S, Itoh S, Tanaka N, et al. A method for detecting myocardial abnormality by using a total current-vector calculated from ST-segment deviation of a magnetocardiogram signal. *Med Biol Eng Comput* 2001; **39**: 21-28.

11. Chen J, Thomson PD, Nolan V, and Clarke J. Age and sex dependent variations in the normal magnetocardiogram compared with changes associated with ischemia. *Ann Biomed Eng* 2004; **32**: 1088-99.

12. Kwong JSW, Leithäuser B, Park JW, and Yu CM. Diagnostic value of magnetocardiography in coronary artery disease and cardiac arrhythmias: A review of clinical data. *Int J Cardiol* 2013; **167**: 1835-42.

13. Page MJ, McKenzie JE, Bossuyt PM, et al. The PRISMA 2020 statement: an updated guideline for reporting systematic reviews. *BMJ*. 2021; **1**: n71.

14. Steinberg BA, Roguin A, Watkins III SP, Hill P, Fernando D, and Resar JR. Magnetocardiogram recordings in a nonshielded environment—reproducibility and ischemia detection. *Ann Noninvasive Electrocardiol* 2005; **10**: 152-60.

15. Coriasso N, Takla RB, Rodriguez D, Pearson C, Pena M, and Daher E. A Novel Way to Predict Obstructive Coronary Artery Disease Requiring Revascularization: The Use of Magnetocardiography. *Circulation* 2021; **144** (suppl 1): A10642 (abstr).
16. Huang X, Hua N, Li L, and Tang F. The value of low temperature superconducting magnetocardiography in the early diagnosis of coronary. *Chin J Evid Based Cardiovasc Med* 2019; **11**: 960-63.
17. Quan W and Lu G. Magnetocardiography changes in coronary artery disease patients without normal or unspecialized resting electrocardiogram. *Chin J Cardiol* 2006; **34**: 500-03.
18. Zhao D, Chen Y, Liu F, Wang J, Zhao C, and Chen Q. The clinical application of magnetocardiography in diagnosis of coronary heart disease. *Journal of Tianjin medical university* 2010; **16**: 242-44.
19. Zhang T, Tang F, Hua N, and Zhang C. Comparison of MCG and coronary angiography in the diagnosis of coronary artery disease. *China medical equipment* 2009; **24**: 11-12.
20. Du X, Li F, Cao J, Li Y, Li Y, Shen Y, et al. The clinical value of magnetocardiography in diagnosis of coronary heart diseases. *Chin J Geriatr Heart Brain Vessel Dis* 2006; **8**: 90-92.
21. Lin L, Tang F, Hua N, Lu H, and Tang X. Contrast study of sensitivity and specificity between magnetocardiography and electrocardiogram in early diagnosis of coronary artery disease in patients with acute chest pain. *Chin Heart J* 2015; **27**: 606-08.
22. Zhao C, Chen Y, Zhao D, Wang J, and Chen Q. Comparison between

magnetocardiography and myocardial perfusion imaging in the diagnosis of myocardial ischemia in patients with coronary artery disease. *Int J Clin Exp Med* 2019; **12**: 13127-34.

23. Wu YW, Lee CM, Liu YB, Wang SS, Huang HC, Tseng WK, et al. Usefulness of magnetocardiography to detect coronary artery disease and cardiac allograft vasculopathy. *Circ J* 2013; **77**: 1783-90.

24. Wu YW, Lin LC, Tseng WK, Liu YB, Kao HL, Lin MS, et al. QTc heterogeneity in rest magnetocardiography is sensitive to detect coronary artery disease: in comparison with stress myocardial perfusion imaging. *Acta Cardiol Sin* 2014; **30**: 445-54.

25. Shin ES, Lam YY, Her AY, Brachmann J, Jung F, and Park JW. Incremental diagnostic value of combined quantitative and qualitative parameters of magnetocardiography to detect coronary artery disease. *Int J Cardiol* 2017; **228**: 948-52.

26. Shin ES, Chung JH, Park SG, Saleh A, Lam YY, Bhak J, et al. Comparison of exercise electrocardiography and magnetocardiography for detection of coronary artery disease using ST-segment fluctuation score. *Clin Hemorheol Microcirc* 2019; **73**: 283-91.

27. Chaikovsky I, Hailer B, Sosnytsky V, Lutay M, Mjasnikov G, Kazmirchuka A, et al. Predictive value of the complex magnetocardiographic index in patients with intermediate pretest probability of chronic coronary artery disease: results of a two-center study. *Coronary Artery Dis* 2014; **25**: 474-84.

28. Chaikovsky I, Mjasnikov G, Lutay M, Udovichenko E, Popov A, Sofienko S, et al.

Coronary artery disease versus coronary microvascular disease: advanced analysis of magnetocardiographic maps. *J Am Coll Cardiol* 2017; **70** (suppl C): GW28-e0528 (abstr).

29. Park JW, Leithäuser B, Vršansky M, and Jung F. Dobutamine stress magnetocardiography for the detection of significant coronary artery stenoses—a prospective study in comparison with simultaneous 12-lead electrocardiography. *Clin Hemorheol Microcirc* 2008; **39**: 21-32.

30. Kanzaki H, Nakatani S, Kandori A, Tsukada K, and Miyatake K. A new screening method to diagnose coronary artery disease using multichannel magnetocardiogram and simple exercise. *Basic Res Cardiol* 2003; **98**: 124-32.

31. Agarwal R, Saini A, Alyousef T, and Umscheid CA. Magnetocardiography for the diagnosis of coronary artery disease—a systematic review and meta-analysis. *Ann Noninvasive Electrocardiol* 2012; **17**: 291-98.

Tables

Table 1

	Coun	Pat.	CHD	Inclusion criteria	Exclusion	Positivity
	/Reg.	num.	prev.		criteria	criteria
Kanzaki <i>et al.</i> (2003) ³⁰	JPN	30	57%	HAP indicated for CAG; healthy volunteers.	/	Maximal QRS IC \geq 0.44.
Park <i>et al.</i> (2005) ⁷	DEU	185	77%	HAP, petrosternal pain, temporary STE/FTW/ITW.	AMI; HUP; registry refusal.	Experienced reader.
Steinberg <i>et al.</i> (2005) ¹⁴	USA	29	66%	HAP, suspected CHD.	Poor-quality data.	Evaluating score \geq 49.
Du <i>et al.</i> (2006) ²⁰	CHN	90	51%	HAP, chest pain; \geq 26 yo..	HF; AF; BBB; LVH; EI.	With 3 MFM indicators.
Quan <i>et al.</i> (2006) ¹⁷	CHN	222	63%	HAP, chest pain, normal ECHO, X-rays and ECG.	HF; BBB; AF; CM; VHD; VH; LVD.	CVEI in -100 ~ 0.
Park <i>et al.</i> (2008) ²⁹	DEU	100	42%	HAP, SAP/ED, 10~90% CAD PTP; \geq 18 yo..	ACS; HOCM; HNOCM; DCM; BBB; pregnancy; ...	With ECD indicators.

Zhang <i>et al.</i> (2009) ¹⁹	CHN	110	63%	HAP, chest pain, normal ECG, Trop I \leq 0.16 ng/L,	MI; HTN; VD; DM; AVB; BBB; IVB; PI; LVEF \leq 50%; ...	\geq 3 abnormal indicators.
Zhao <i>et al.</i> (2010) ¹⁸	CHN	493	78%	HAP, suspected CHD.	HTN; FAPB; CBBB; VPB; AMI; VH; DCM; ...	\geq 3 abnormal indicators.
Wu <i>et al.</i> (2013) ²³	TWN	75	68%	HAP, suspected CHD.	AR; MI history; UAP; VHD; MP; ...	QTc dispersion \geq 79 ms or SI- QTc \geq 9 ms.
Chaikovsky <i>et al.</i> (2014) ²⁷	UKR, DEU	79	68%	HAP, chest pain.	MI history; AF; AFL; HF; PI; abnormal ECG; ...	Complex index \geq 10.
Wu <i>et al.</i> (2014) ²⁴	TWN	55	66%	HAP, chest pain, SR, intermediate CAD PTP.	AR; recent MI; UAP; MP; LVEF \leq 50%; ...	QTc dispersion \geq 79 ms or SI- QTc \geq 9.1 ms.
Lin <i>et al.</i> (2015) ²¹	CHN	287	66%	HAP, chest pain.	VAP; persistent STE; BBB; AR;	\geq 3 abnormal indicators.

LVH.

Chaikovsky
et al. DEU 136 60% HAP, chest pain. / With 32 CDV features
(2017)²⁸

Shin *et al.*, DEU 96 48% HAP, indicated ACS; AMI; Non-dipole
(2017)²⁵ for CAG, >18 CABG; CTCO; phenomeno.
yo., ... VHD; ESRF; ...

Zhao *et al.* CHN 104 31% HAP, diagnosed HTN; AR; AMI; ≥ 2 abnormal
(2019)²² with MCG, MPI VH/DCM; ... indicators.
and CAG.

Shin *et al.* DEU 202 39% HAP, indicated ACS; AMI; ST-segment
(2019)²⁶ for CAG, >18 CABG; CTCO; fluctuation
yo., ... VHD; ESRF; ... score
change ≥ -40.0
%

Huang *et al.* CHN 213 62% HAP, suspected MT; SHD; ≥ 1 abnormal
(2019)¹⁶ CHD. VHD; CM; MA. indicators.

Coriasso *et al.* (2021)¹⁵ USA 65 42% HAP, suspected / With 3 MFM
CHD. features.

ACS, acute coronary syndromes; AF, atrial fibrillation; AFL, atrial flutter; AMI, acute myocardial infarction; AP, angina pectoris; AR, arrhythmias; AVB, atrioventricular block; BBB, bundle branch block; CABG, coronary artery bypass surgery; CAG, coronary angiography; CBBB, complete bundle branch block; CDV, current density vector; CK-MB, creatine kinase-MB isoenzyme; CM, cardiomyopathy; CTCO, chronic total coronary occlusion; CVEI, complex ventricular excitation index; DCM, dilated cardiomyopathy; DM, diabetes mellitus; ECD, epicardial current density; ECHO, echocardiography; ED, exertional dyspnea; EI, electrolyte imbalance; ESRF, end stage renal failure; FAPB, frequent atrial premature beats; FTW, flat T wave; HAP, hospital-admitted patient; HF, heart failure; HNOCM, hypertrophic nonobstructive cardiomyopathy; HOCM, hypertrophic obstructive cardiomyopathy; HTN, hypertension; HUP, hemodynamically unstable patient; IC, integral change; IHD, ischemic heart disease; ITW, inverted T wave; IVB, intraventricular block; LV, left ventricular; LVD, left ventricular dysfunction; LVEF, left ventricular ejection fraction; MA, malignant arrhythmias; MD, magnetic dipole; MFM, magnetic field map; MI, myocardial infarction; MP, metallic prosthesis; MPI, myocardial perfusion imaging; MT, malignant tumor; PA, pre-peak repolarization angle; PAD, pre-peak repolarization angular deviation; PCI, percutaneous coronary intervention; PI, pacemaker implantation; PoA, post-peak repolarization angle; PoAD, post-peak repolarization angular deviation; PoT, post-peak repolarization trajectory; PPAC, pre-post angle change; PT, pre-peak repolarization trajectory; PTP, pre-test probability; SAP, stable angina pectoris; SHD, structural heart disease; SI-QTc, smooth index QTc; SR, sinus rhythm; STE, ST-segment elevation; UAP, unstable angina pectoris; VAP, variant angina pectoris; VD, valve disease; VH, ventricular hypertrophy; VHD, valvular heart disease; VPB, ventricular premature beats; yo., years old.

Table 1 Characteristics of included studies.

Table 2

	Risk of Bias				Applicability Concerns		
	Patient Selection	Index Test	Reference Standard	Flow and timing	Patient Selection	Index Test	Reference Standard
Kanzaki <i>et al.</i> (2003) ³⁰	High	High	Unclear	Unclear	Low	Low	Low
Park <i>et al.</i> (2005) ⁷	Unclear	Unclear	Low	High	Low	Low	Low
Steinberg <i>et al.</i> (2005) ¹⁴	Unclear	Low	Unclear	Low	Low	Low	Low
Du <i>et al.</i> (2006) ²⁰	Unclear	Unclear	Low	Unclear	Low	Low	Low
Quan <i>et al.</i> (2006) ¹⁷	Unclear	Unclear	Unclear	Unclear	Low	Low	Low
Park <i>et al.</i> (2008) ²⁹	Low	Unclear	Unclear	Low	Low	Low	Low
Zhang <i>et al.</i> (2009) ¹⁹	Unclear	Unclear	Unclear	Low	Low	Low	Low
Zhao <i>et al.</i> (2010) ¹⁸	Unclear	Unclear	Unclear	Unclear	Low	Low	Low
Wu <i>et al.</i> (2013) ²³	Unclear	High	Unclear	Low	Low	Low	Low

Chaikovsky <i>et al.</i> (2014) ²⁷	Unclear	High	Unclear	Unclear	Low	Low	Low
Wu <i>et al.</i> (2014) ²⁴	Unclear	High	Unclear	Low	Low	Low	Low
Lin <i>et al.</i> (2015) ²¹	Unclear	Unclear	Unclear	Unclear	Low	Low	Low
Chaikovsky <i>et al.</i> (2017) ²⁸	Unclear	Unclear	Unclear	Unclear	Low	Low	Low
Shin <i>et al.</i> , (2017) ²⁵	Unclear	High	Unclear	Low	Low	Low	Low
Zhao <i>et al.</i> (2019) ²²	Low	Unclear	Unclear	Unclear	Low	Low	Low
Shin <i>et al.</i> (2019) ²⁶	Unclear	High	Unclear	Unclear	Low	Low	Low
Huang <i>et al.</i> (2019) ¹⁶	Unclear	High	Unclear	Unclear	Low	Low	Low
Coriasso <i>et al.</i> (2021) ¹⁵	Unclear	Unclear	Unclear	Unclear	Low	Low	Low

Table 2 Quality evaluation. The names of each study are labeled on the left side. It encompasses the assessment of risk of bias and applicability across seven dimensions, which are evaluated on three levels: high, low, and unclear.

Table 3

	Number of		Sensitivity		Specificity		
	Studies	Samples	Value (95% CI)	p-value	Value (95% CI)	p-value	
Rest	Silent	4	441	0.84 (0.71-0.97)	0.09	0.82 (0.68-0.97)	0.43
	ECG Ensemble	14	2130	0.87 (0.81-0.93)		0.79 (0.70-0.87)	
Stress test	Yes	4	428	0.86 (0.74-0.99)	0.21	0.87 (0.76-0.97)	0.71
	No	14	2143	0.86 (0.80-0.92)		0.77 (0.68-0.85)	
Ref-std.	Mild	7	1270	0.89 (0.83-0.96)	0.01	0.78 (0.67-0.90)	0.13
	Severe	10	1236	0.86 (0.78-0.93)		0.78 (0.68-0.88)	

Table 3 The results of meta-regression and subgroup analysis. The sensitivity for diagnosing early CHD and severe CHD performs significant difference ($P < 0.05$). Ref-std., reference

standard.

Figures with Figure Legends

Figure 1 Results of study inclusion.

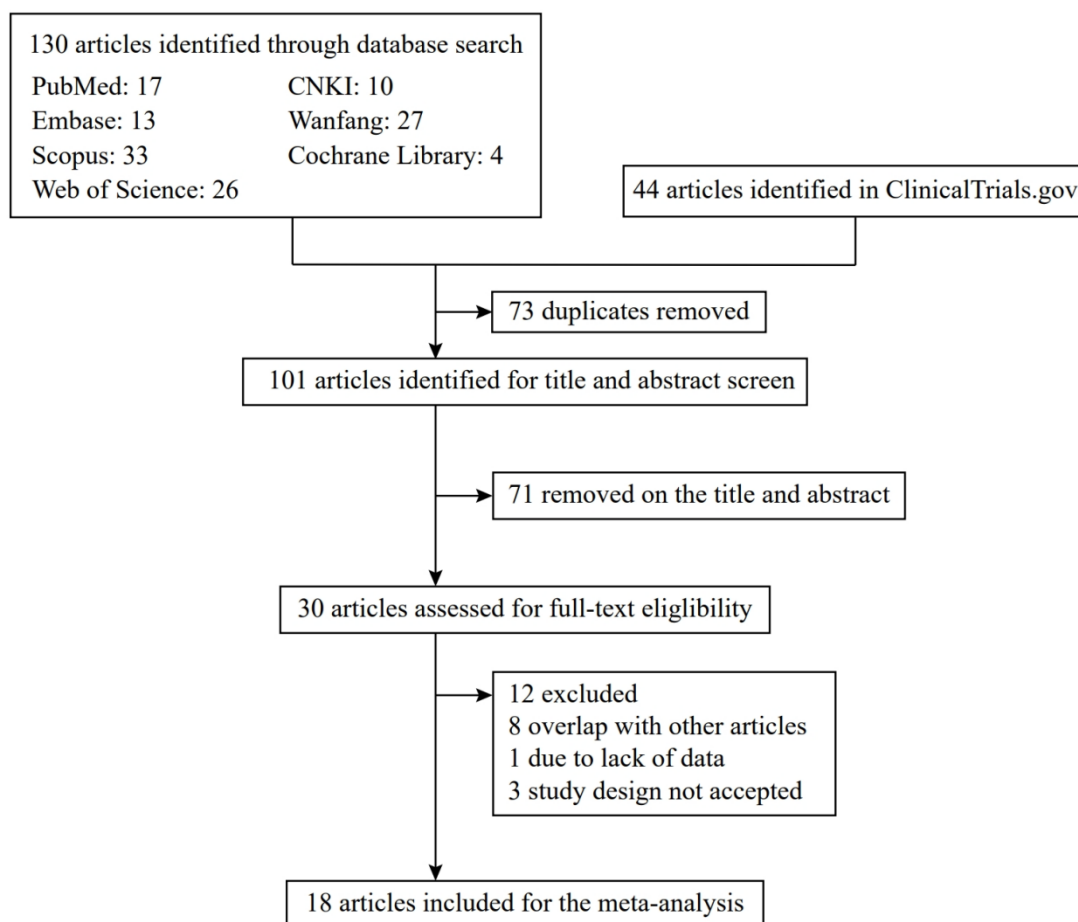


Figure 2 The forest plot showing the results of individual studies and their combination. The left subfigure calculates the sensitivity, and the right subfigure calculates the false positive rate. Each row in the subfigure represents a study, with the study name and the numbers of samples in diagnostic 2×2 table. The confidence interval and prediction interval for the combined index are shown at the bottom of each subfigure. The combined sensitivity of MCG for diagnosing CHD is 0.86 (0.80 – 0.91), and the combined specificity is 0.79 (0.71 – 0.86). The value of Cochran's Q for sensitivity and specificity are 294.11 and 154.26, respectively. The value of I^2 for sensitivity and specificity are 94.22% (92.48 – 95.96) and 88.98% (84.95 – 93.01), respectively.

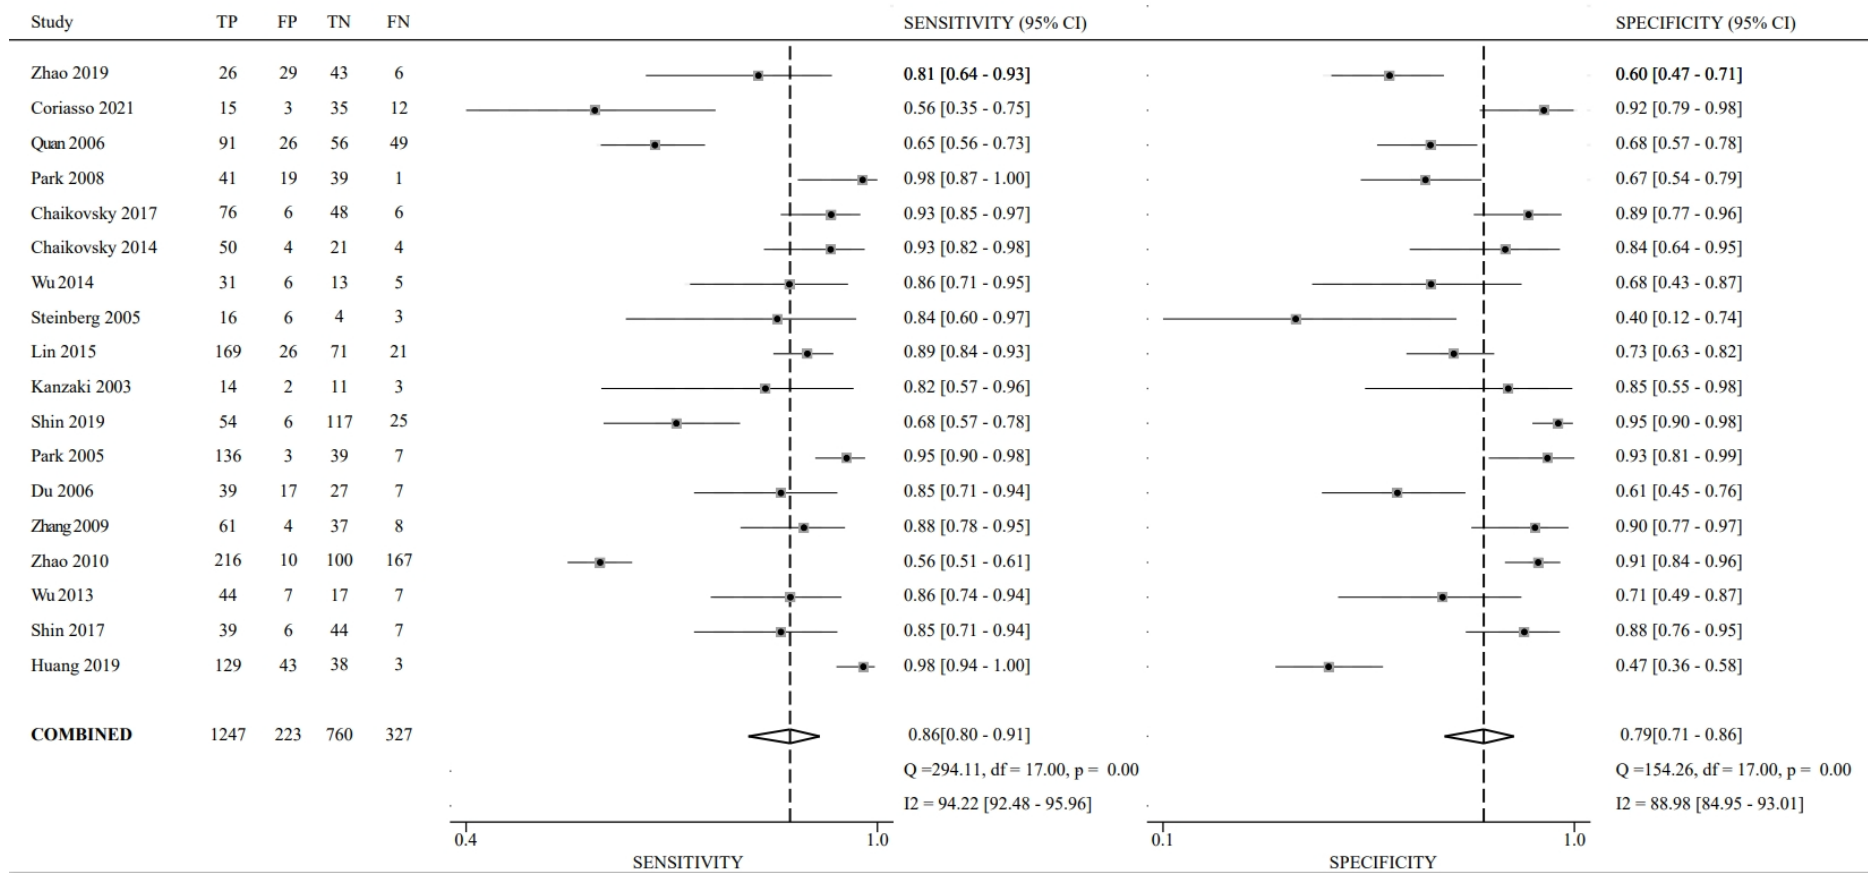


Figure 3 The combined results of all studies. Each red circle represents an included study, and the size of it indicates the sample size. The black line is the SROC curve, and the red star represents the summary point obtained by combination, corresponding to a sensitivity of 0.86 and a specificity of 0.79. The blue and gray dashed lines represent the confidence interval and prediction interval of the total characteristics.

