

Technical Development and In Silico Implementation of SyntheticMR in Head and Neck Adaptive Radiation Therapy: A Prospective R-IDEAL Stage 0/1 Technology Development Report

Lucas McCullum^{1,2}, Samuel Mulder^{1,2}, Natalie West^{1,2}, Robert Aghoghovbia³, Alaa Mohamed Shawky Ali², Hayden Scott^{1,2}, Travis C. Salzillo⁴, Yao Ding⁴, Alex Dresner⁵, Ergys Subashi⁴, Dan Ma⁶, R. Jason Stafford⁷, Ken-Pin Hwang⁷, Clifton D. Fuller²

¹UT MD Anderson Cancer Center UTHealth Houston Graduate School of Biomedical Sciences, Houston, USA

²Department of Radiation Oncology, The University of Texas MD Anderson Cancer Center, Houston, TX, USA

³Morehouse School of Medicine, Atlanta, USA

⁴Department of Radiation Physics, The University of Texas MD Anderson Cancer Center, Houston, TX, USA

⁵Philips Healthcare MR Oncology, Cleveland, Ohio, USA

⁶Department of Biomedical Engineering, Case Western Reserve University, Cleveland, Ohio, USA

⁷Department of Imaging Physics, The University of Texas MD Anderson Cancer Center, Houston, TX, USA

Corresponding Author: Clifton D. Fuller <cdfuller@mdanderson.org>

Keywords: SyntheticMR, SyMRI, MRI, Quantitative Imaging, MR-Linac, Radiotherapy, Radiation Therapy, Adaptive Radiation Therapy, Head and Neck Cancer

Contributor Roles Taxonomy (CRediT) Attribution Statement: *Conceptualization:* L.M. and C.D.F.; *Data curation:* L.M. and K.H.; *Formal analysis:* L.M.; *Funding acquisition:* C.D.F.; *Investigation:* L.M., S.J.M., N.W. and T.C.S.; *Methodology:* L.M. and C.D.F.; *Project administration:* C.D.F.; *Resources:* L.M., S.J.M., N.W., R.A., A.M., H.S., T.C.S., Y.D., E.S., K.H. and C.D.F.; *Software:* L.M.; *Supervision:* A.D., E.S., D.M., R.J.S., K.H. and C.D.F.; *Validation:* L.M., S.J.M. and N.W.; *Visualization:* L.M.; *Writing – original draft:* L.M.; *Writing - review & editing:* L.M., S.J.M., N.W., R.A., A.M., H.S., T.C.S., Y.D., A.D., E.S., D.M., R.J.S., K.H. and C.D.F.

IRB Statement: All participants provided written informed consent. Volunteers were consented to an internal volunteer imaging protocol (PA15-0418), both approved by the institutional review board at The University of Texas MD Anderson Cancer Center.

Conflicts of Interest: AD has received related research support from Elekta AB and unrelated royalties / licenses from Resoundant LLC. KH has received related investigational software / research support from SyntheticMR AB and unrelated research support from GE Healthcare. CDF has received related travel, speaker honoraria and/or registration fee waiver from: Elekta

AB and unrelated travel, speaker honoraria and/or registration fee waiver from: The American Association for Physicists in Medicine; the University of Alabama-Birmingham; The American Society for Clinical Oncology; The Royal Australian and New Zealand College of Radiologists; The American Society for Radiation Oncology; The Radiological Society of North America; and The European Society for Radiation Oncology. CDF has received related direct industry grant/in-kind support, honoraria, and travel funding from Elekta AB and has served in an unrelated consulting capacity for Varian/Siemens Healthineers, Philips Medical Systems, and Oncospace, Inc.

Funding Statement: LM is supported by a National Institutes of Health (NIH) Diversity Supplement (R01CA257814-02S2). SM is supported by a training fellowship from UTHealth Houston Center for Clinical and Translational Sciences TL1 Program (Grant No. TL1 TR003169). NW is supported by a NIH National Institute of Dental and Craniofacial Research (NIDCR) Academic Industrial Partnership Grant (R01DE028290). RA is supported through the University of Texas MD Anderson Cancer Center Division of Radiation Oncology and The Sterling Foundation. TCS is supported by The University of Texas Health Science Center at Houston, the Center for Clinical and Translational Sciences TL1 Program (TL1TR003169). DM is supported by the National Cancer Institute (NCI) (R01CA269604, R01CA282516, and R01CA292091). CDF has received unrelated funding and salary support from: NIH National Institute of Dental and Craniofacial Research (NIDCR) Academic Industrial Partnership (R01DE028290), the Administrative Supplement to Support Collaborations to Improve AIML-Readiness of NIH-Supported Data (R01DE028290-04S2); NIDCR Establishing Outcome Measures for Clinical Studies of Oral and Craniofacial Diseases and Conditions award (R01DE025248); NSF/NIH Interagency Smart and Connected Health (SCH) Program (R01CA257814); NIH National Institute of Biomedical Imaging and Bioengineering (NIBIB) Research Education Programs for Residents and Clinical Fellows Grant (R25EB025787); NIH NIDCR Exploratory/Developmental Research Grant Program (R21DE031082); NIH/NCI Cancer Center Support Grant (CCSG) Pilot Research Program Award from the UT MD Anderson CCSG Radiation Oncology and Cancer Imaging Program (P30CA016672); Patient-Centered Outcomes Research Institute (PCS-1609-36195) sub-award from Princess Margaret Hospital; National Science Foundation (NSF) Division of Civil, Mechanical, and Manufacturing Innovation (CMMI) grant (NSF 1933369). CDF receives grant and infrastructure support from MD Anderson Cancer Center via: the Charles and Daneen Stiefel Center for Head and Neck Cancer Oropharyngeal Cancer Research Program; the Program in Image-guided Cancer Therapy; and the NIH/NCI Cancer Center Support Grant (CCSG) Radiation Oncology and Cancer Imaging Program (P30CA016672).

Data Availability Statement: All relevant anonymized SyntheticMR unprocessed (pre-SyMRI) DICOM files are to be made publicly available after manuscript acceptance at the following DOI: 10.6084/m9.figshare.26835715. The accompanying code for image visualization and statistical analysis will be made publicly available at the following URL: https://github.com/Lucas-Mc/SyntheticMR_R-IDEAL_0-1.

Acknowledgements: The authors would like to thank SyntheticMR AB for their assistance in the formal data analysis through their software, SyMRI.

Abstract

Objective: The purpose of this study was to investigate the technical feasibility of integrating the quantitative maps available from SyntheticMR into the head and neck adaptive radiation oncology workflow. While SyntheticMR has been investigated for diagnostic applications, no studies have investigated its feasibility and potential for MR-Simulation or MR-Linac workflow. Demonstrating the feasibility of using this technique will facilitate rapid quantitative biomarker extraction which can be leveraged to guide adaptive radiation therapy decision making.

Approach: Two phantoms, two healthy volunteers, and one patient were scanned using SyntheticMR on the MR-Simulation and MR-Linac devices with scan times between four to six minutes. Images in phantoms and volunteers were conducted in a test/retest protocol. The correlation between measured and reference quantitative T1, T2, and PD values were determined across clinical ranges in the phantom. Distortion was also studied. Contours of head and neck organs-at-risk (OAR) were drawn and applied to extract T1, T2, and PD. These values were plotted against each other, clusters were computed, and their separability significance was determined to evaluate SyntheticMR for differentiating tumor and normal tissue.

Main Results: The Lin's Concordance Correlation Coefficient between the measured and phantom reference values was above 0.98 for both the MR-Sim and MR-Linac. No significant levels of distortion were measured. The mean bias between the measured and phantom reference values across repeated scans was below 4% for T1, 7% for T2, and 4% for PD for both the MR-Sim and MR-Linac. For T1 vs. T2 and T1 vs. PD, the GTV contour exhibited perfect purity against neighboring OARs while being 0.7 for T2 vs. PD. All cluster significance levels between the GTV and the nearest OAR, the tongue, using the SigClust method was $p < 0.001$.

Significance: The technical feasibility of SyntheticMR was confirmed. Application of this technique to the head and neck adaptive radiation therapy workflow can enrich the current quantitative biomarker landscape.

1. Introduction

Magnetic resonance imaging (MRI) plays a vital role in visualizing tissues which are often indistinguishably isointense on computed tomography (CT)¹. This becomes especially important in the field of radiation oncology due to most malignancies being in the soft tissue where CT has lower contrast. Due to this superiority, systems designed for radiation therapy (i.e., the linear accelerator, or Linac) have integrated diagnostic-level MRIs to create the 1.5T MR-Linac², allowing for simultaneous radiation therapy delivery and MRI acquisition for anatomically dynamic structures (i.e., the lung). Furthermore, due to the availability of imaging acquired at each treatment fraction, strategies to adapt the treatment delivery based on imaging changes have gained traction and is known as adaptive radiation therapy, or ART.

However, unlike CT, the radiation therapy workflow in MRI is currently focused around qualitative rather than quantitative representations of tumor and healthy tissue using the on-board MRI system of the MR-Linac. Though easy to interpret visually, the arbitrary signal values associated with standard relaxation “weighted” images in MRI present hurdles to the standard radiation therapy workflow, not the least of which are that these images are not ideal to monitor treatment response since they do not provide consistent quantitative measurements which can be compared across the different fractions of treatment³. In head and neck cancer, quantitative MRI probing tissue T1 and T2 properties has recently been investigated for diagnosis⁴, assessment of treatment response⁵, and assessment of normal tissue damage⁶. However, on the 1.5T MR-Linac, T1 and T2 mapping has been limited to acquisition times of exceeding 3 minutes and 5 minutes, respectively^{7,8}. Therefore, acquiring T1 and T2 maps alone will require upwards of 8 minutes and suffer from higher misregistration error due to the potential for patient adjustments intra- and inter-scan. This time requirement is critical on the MR-Linac where, typically, less than 10 minutes are available for elective imaging within the clinical workflow⁹, and this will only decrease as broader patient coverage is demanded with the recently introduced Comprehensive Motion Management (CMM) software¹⁰.

The company SyntheticMR (Linköping, Sweden) has developed a single scan time (i.e., <6 minutes) simultaneous multiparametric MRI acquisition sequence originally known as QRAPMASTER¹¹ and more regularly known as multi-dynamic multi-echo (MDME) on Siemens MRI scanners, MAGiC on GE scanners, and SyntAc on Philips scanner. Through their post-processing software, SyMRI, these acquired images can be reconstructed to quantitative T1, T2, and proton density (PD) maps and derivative synthetic contrast maps such as T1/T2/PD-weighted and inversion recovery (IR), e.g., fluid attenuated (FLAIR), phase-sensitive (PSIR), and short inversion time (STIR). The most common implementation of the sequence is the 2D-MDME^{11–13} which acquires multiple 2D slices, often with slice thicknesses of 3 – 6 mm while in-plane resolution is often <2 mm. However, a 3D version of the sequence capable of 1 mm isotropic acquisitions (3D-QALAS)¹⁴, has been developed and has shown clinically acceptable quantitative accuracy and repeatability in a multi-center¹⁵ and multi-vendor study¹⁶. More details of the MR physics, technical considerations, and pulse sequence design can be seen in the review article by Hwang et al. 2022¹⁷.

SyntheticMR has seen increasing usage for diagnostic imaging^{18–21}, however limited investigation has been conducted in usage for radiation oncology^{22–25} and even fewer studies have focused on the head and neck^{26,27}. Further, no studies to the author’s knowledge have

evaluated the technical feasibility of the SyntheticMR sequence on MR-Simulation (MR-Sim) or MR-Linac devices. The potential application of SyntheticMR to the radiation oncology space has high promise for increasing the dimensionality available for treatment monitoring and optimal adaptive therapy decisions. Specifically, within the head and neck oncology space, due to the large number of organs-at-risk (OARs) near the target, advanced quantitative MRI techniques would be advantageous to characterize simultaneous normal tissue dose-responses and tumor control more effectively. Therefore, the purpose of this study is to investigate the technical feasibility of integrating SyntheticMR into the head and neck adaptive radiation therapy workflow on both an MR-Sim and MR-Linac scanner. This will be presented using the radiotherapy-predicate studies, idea, development, exploration, assessment, and long-term study (R-IDEAL) framework, as recommended by the MR-Linac Consortium, completing Stage 0 (radiotherapy predicate studies) and Stage 1 (first time use) systematic evaluations²⁸.

2. Methods and Materials

2.1. MRI Acquisition Parameters

To evaluate SyntheticMR across the radiation oncology department, MRI scans were performed on a 3T Siemens Vida MR-Sim scanner (Siemens Healthcare; Erlangen, Germany) and a 1.5T MR-Linac (Unity; Elekta AB; Stockholm, Sweden). For this study, the 2D-MDME sequence was acquired with acquisition parameters as shown in Table 1. These parameters were chosen to optimize the acquisition for different clinical scenarios on the MR-Linac including the possibility for lymph node evaluation²⁹ (coarse sequence) and required resolution for stereotactic radiation therapy precision³⁰ (fine sequence). Further, due to the non-isotropic acquisition of 2D-MDME, all scans were acquired in the axial / transverse orientation to best visualize structures in the head and neck at all points in the radiation therapy workflow^{31,32}.

Table 1. Acquisition parameters across all scanners utilized in this study.

	3T Siemens Vida	1.5T Elekta Unity (coarse sequence)	1.5T Elekta Unity (fine sequence)
Software Version	XA50	R5.7.1.2	R5.7.1.2
Field-of-View (mm³)	256 x 256 x 149	250 x 349 x 199	256 x 256 x 179
Acq. Voxel Size (mm³)	1.00 x 1.67	2.02 x 2.65	1.00 x 1.03
Recon. Voxel Size (mm³)	0.5 x 0.5	0.99 x 0.99	0.5 x 0.5
Slice Thickness (mm)	4	3	4
Slice Gap (mm)	1	1	1
Number of Slices	30	50	36
TR / TE₁ / TE₂ (ms)	4330 / 19 / 94	8599 / 11 / 102	6191 / 12 / 112
Echo Train Length (ETL)	12	12	12
Acceleration (GRAPPA / CS-SENSE)	3	3	3
Refocusing Flip Angle (°)	150	180	180
Acquisition Time (m:ss)	4:06	4:44	5:53

2.2. MR Phantoms Assessed

The American College of Radiology (ACR) large phantom was used to evaluate geometric distortion and accuracy. The CaliberMRI “ISMRM/NIST” Premium System Phantom Model 130 phantom (CaliberMRI; Boulder, CO) was used as a reference for NIST-traceable T1, T2, and PD values³³. This phantom includes 14 vials for each metric (42 total vials) suitable for T1 values between 20 and 1724 ms, T2 values between 9 and 853 ms, and PD values between 5 and 100% at 20°C on a 1.5T MRI scanner. This was confirmed during routine quality assurance that the temperature inside the bore averaged 20°C with minimal fluctuations. Reference values are also provided by the CaliberMRI for 3T MRI scanners. To evaluate repeatability, two repetitions in phantom were performed in a test-retest method using a coronal slice orientation. Similarly, to evaluate reproducibility, this process was reproduced across both the MR-Sim and MR-Linac scanners.

2.3. Healthy Volunteer and Patient Description

Two healthy volunteers were imaged on both the MR-Sim and MR-Linac and assigned the designation of Volunteer 1 (20s-year-old male) and Volunteer 2 (20s-year-old female) for future comparisons. Additionally, a 50s-year-old male with American Joint Committee on Cancer (AJCC) 8th Edition Stage I (cT2, cN0, cM0, p16+) human papilloma virus (HPV) positive of oropharynx, squamous cell carcinoma of the left tonsil was scanned on the MR-Sim to evaluate the potential of SyntheticMR in the radiation therapy workflow.

2.4. Data Collection and Image Processing

The images were processed using the SyntheticMR post-processing software, SyMRI (StandAlone 11.3.11, Linköping, Sweden) developed specifically for the 2D-MDME sequence. The geometric accuracy was evaluated using the ACR phantom by measuring four equal radially spaced diameters and comparing them to the expected length of 190 mm to within ± 2 mm³⁴. For the phantom analysis, a circular region-of-interest (ROI) was created in each vial using 3D Slicer³⁵ (<https://www.slicer.org/>) using the synthetically reconstructed T2-weighted MRI and the values within each ROI were extracted for processing in the quantitative T1, T2, and PD maps. A margin of approximately 10% of the vial’s diameter was left to account for ringing artifacts hindering accurate readings³⁶. For the *in vivo* analysis, the parotid and submandibular glands were chosen for analysis as the primary OAR for salivary dysfunction and were contoured automatically using a deep learning algorithm in the Advanced Medical Imaging Research Engine (ADMIRE) research software (v3.48.4, Elekta AB, Stockholm, Sweden). Additional critical structures including the tongue, bilateral infraorbital lymph spaces, mandible, and bilateral masseter muscles were contoured by medical students in RayStation Research 12A R v13.1.100.0 (RaySearch Laboratories, Stockholm, Sweden).

2.5. Statistical Analysis

All relevant analysis concerning statistical methods are formulated using the guidelines for reporting Statistical Analyses and Methods in the Published Literature (SAMPL)³⁷. All computational analysis was completed using Python 3.8.10. To evaluate quantitative parameter accuracy, for each vial inside the ISMRM/NIST phantom, the values inside the ROI were

extracted and the mean and standard deviation were calculated and compared to manufacturer reference values. For all calculations, analysis was restricted to clinical ranges of T1 (250 – 2000 ms), T2 (30 – 300 ms), and PD (20 – 160 pu)³⁸ across both 1.5T and 3T MRI devices. Lin's Concordance Correlation Coefficient (LCCC) was used instead of Pearson's r^2 to evaluate direct agreement to reference values instead of generalized linearity. For measuring bias between the measured values and reference values, the mean bias was determined, and Spearman's rank correlation coefficient (i.e., Spearman's ρ) was calculated to test for significant generalized correlations between bias and the magnitude of the reference value. A p-value of 0.05 was used for statistical significance. These trends were further visualized using a Bland-Altman plot³⁹. Cluster analysis was performed using an elliptical envelope and a soft margin assuming 40% outliers. To assess the separation of the clusters for desired ROIs, the purity measure was used to describe the proportion of desired data points that are within the desired cluster compared to other ROIs. Statistical significance between desired ROIs was calculated using the SigClust method⁴⁰ with soft thresholding and 100 Monte Carlo iterations following mean centering and variance normalization.

3. Results

3.1. Phantom Analysis

For the geometric accuracy / distortion analysis using the ACR large phantom, the MR-Sim and both sequences on the MR-Linac showed within-tolerance agreement with the 190 mm expected diameter for each of the four measurements. Further, lines drawn along the geometry grid lines were straight and showed no intra-phantom distortion.

When evaluating quantitative parameter accuracy, the Lin's Concordance Correlation Coefficient between the measured and phantom reference values was above 0.97 for both the MR-Sim and MR-Linac when analyzing for T1, T2, and PD as shown in Figure 1. The highest agreement was seen in the PD values (average LCCC = 0.995), followed by T1 (average LCCC = 0.987), then T2 (average LCCC = 0.985). There is no significant difference between the LCCC of the MR-Sim and MR-Linac.

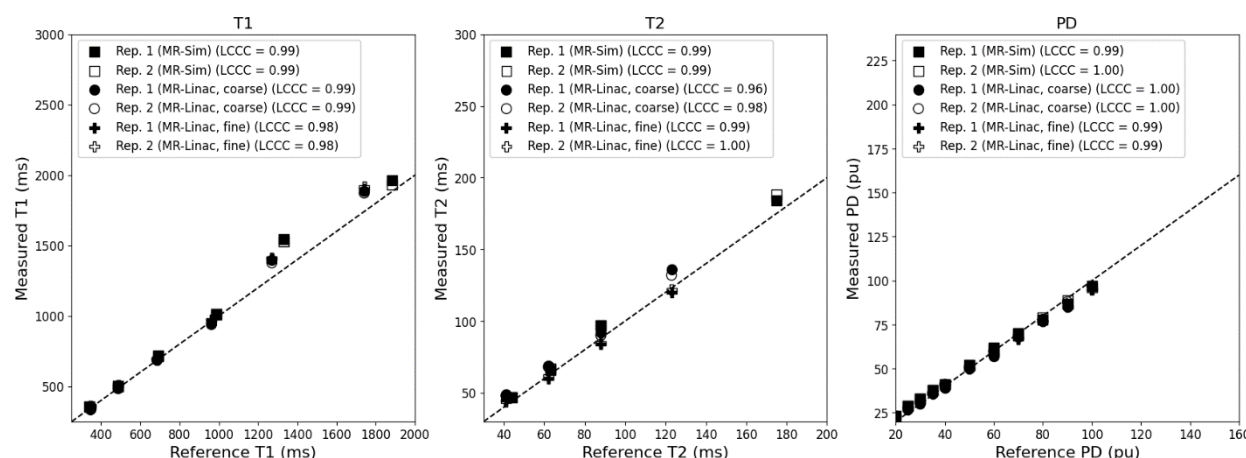


Figure 1. Correlation plot between the measured and reference T1 (left), T2 (center), and PD (right) for the MR-Sim and both coarse and fine sequences for the MR-Linac using a test-retest protocol. Abbreviations: LCCC = Lin's Concordance Correlation Coefficient.

The mean bias between the measured and phantom reference values across both repeat scans was 4.22% for T1, 6.32% for T2, and 3.11% for PD for both the MR-Sim and MR-Linac as shown in Figure 2. The MR-Linac coarse sequence had the lowest average T1 bias at 0.19% while averaging 1.70% for T2 and 9.62% for PD. The MR-Linac fine sequence had the lowest average T2 and PD bias at 0.76% and 1.92%, respectively, while averaging 5.12% for T1. The MR-Sim averaged biases of 5.42% for T1, 7.35% for T2, and 5.62% for PD. When calculating the correlation between reference values and bias, only the PD values showed significant p-values (all $p < 0.001$) with a Spearman rank correlation coefficient averaging -0.96 across the MR-Sim and both sequences on the MR-Linac.

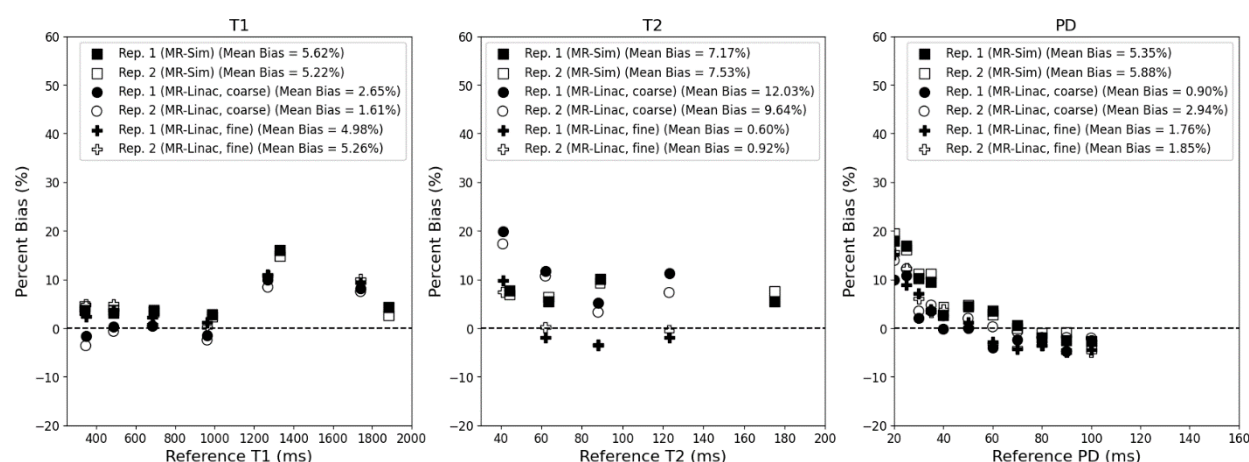


Figure 2. Bland-Altman plot between the measured and reference T1 (left), T2 (center), and PD (right) for the MR-Sim and both coarse and fine sequences for the MR-Linac using a test-retest protocol.

3.2. In vivo Analysis

An example of the SyMRI post-processing generated quantitative and subsequent synthetically generated contrast maps on the head and neck cancer patient on the MR-Sim in Figure 3. Note, the weighted contrast maps can be adjusted to different TE and TR values to achieve seemingly unlimited contrast options. Further, the inversion recovery (IR) sequences can be adjusted in a comparable way through the inversion time (TI).

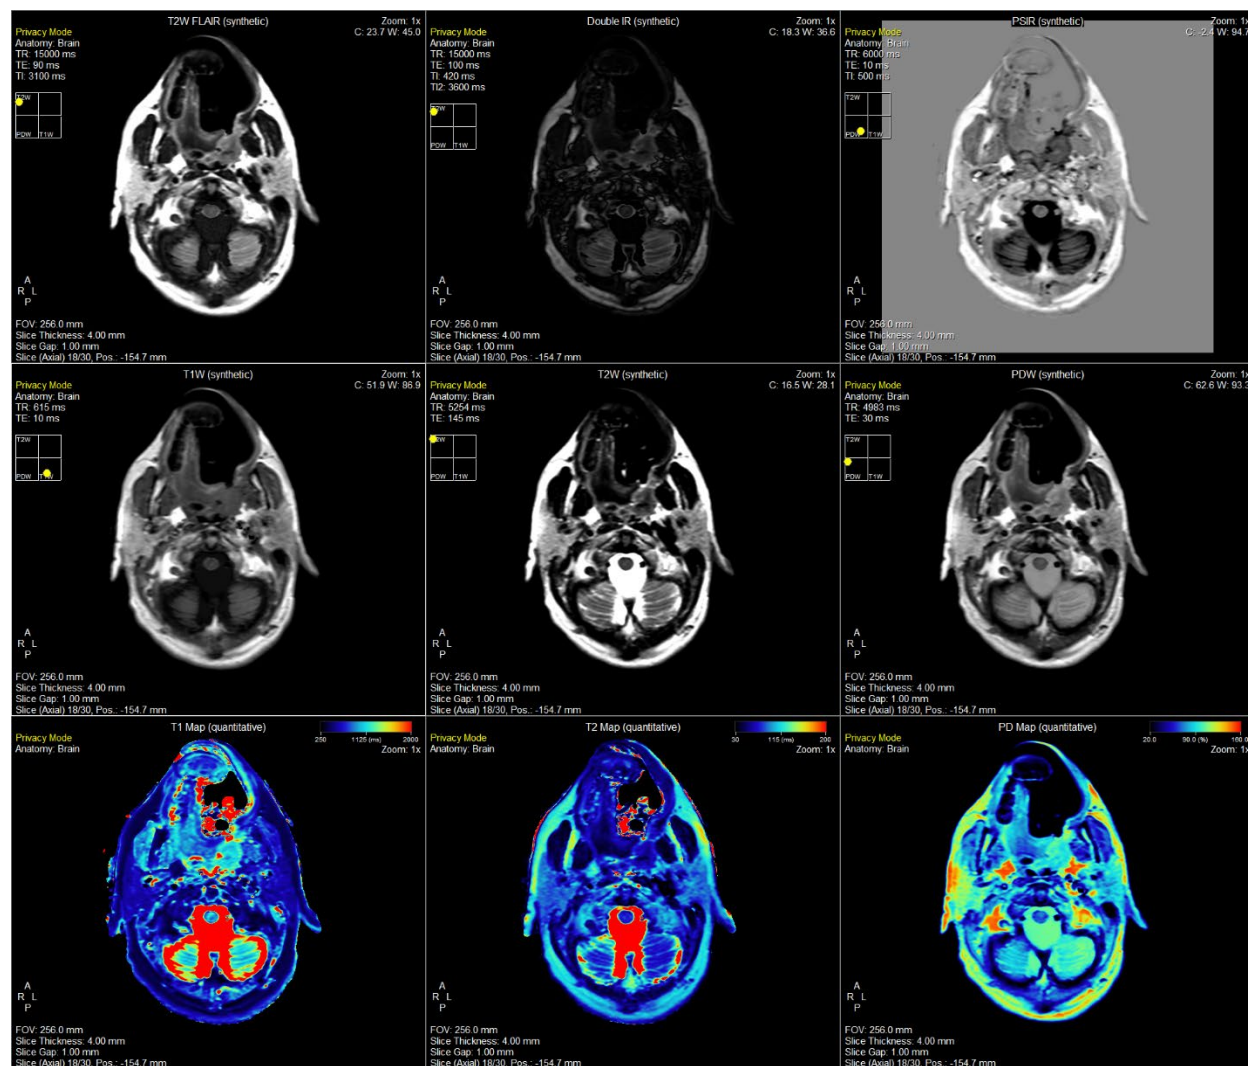


Figure 3. Demonstration of the SyMRI post-processing package offered by SyntheticMR for the head and neck cancer patient on the MR-Sim scanner. Shown here is an axial / transverse slice at the level of the parotid glands, medial pterygoid muscle, and masseter muscle. The same set of images are shown in the Supplementary Materials for Volunteer 1 on the MR-Sim (Figure 3-S1), Volunteer 2 on the MR-Sim (Figure 3-S2), Volunteer 1 on the MR-Linac coarse sequence (Figure 3-S3), and Volunteer 1 on the MR-Linac fine sequence (Figure 3-S4).

For the head and neck cancer patient, the T1, T2, and PD values inside each ROI were extracted and plotted against each other in two dimensions as shown in Figure 4. The purity measure was used between points inside each contour to determine cluster separability between the tumor and neighboring OARs. For T1 vs. T2 and T1 vs. PD, the GTV contour exhibited perfect purity while being 0.7 for T2 vs. PD. All cluster significance levels between the GTV and the nearest OAR, the tongue, using the SigClust method was $p < 0.001$.

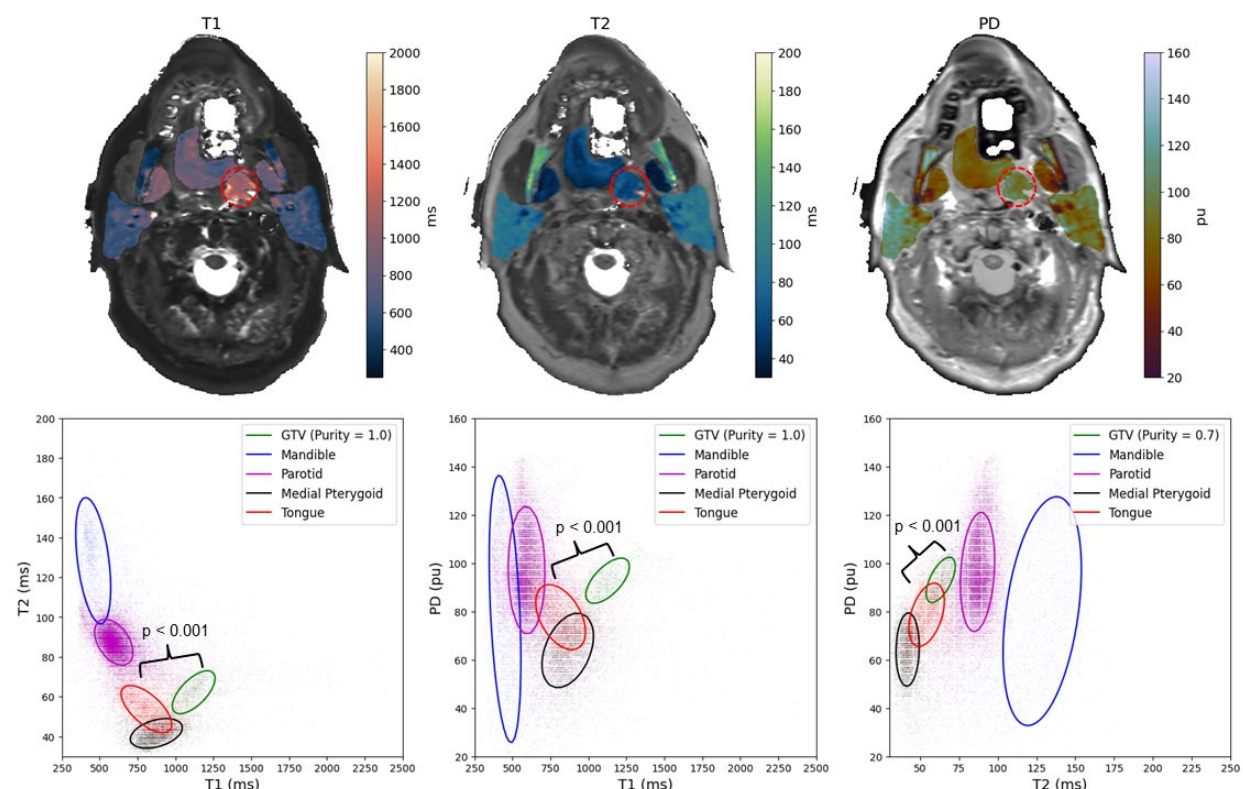


Figure 4. Above, the quantitative spatial maps of neighboring OARs for the patient on the MR-Sim overlaid on top of their respective synthetically generated contrast map. The gross tumor volume (GTV) is shown in red dashed circle. Note, this patient was wearing a bite block and a permanent retainer which caused significant signal dropout in the oral tongue as shown by the white regions. Below, a demonstration of the separation generated by SyntheticMR for differentiating tumor and neighboring healthy tissues. Additional quantitative cluster analysis for more additional OARs in healthy volunteers is shown in Figure 4-S1 of the Supplementary Materials.

4. Discussion

As shown in this technical feasibility analysis, SyntheticMR has the potential to create a paradigm shift in how imaging via MRI is done in the adaptive radiation oncology workflow. When comparing to a prior study collecting T1 and T2 measurements in parotid glands on 1.5T scanners⁴¹, the mean and standard deviation T1, 578.8 (67.9), and T2, 104.5 (11.7), agreed with the distribution shown in this paper. To the author's knowledge, this is the first study investigating SyntheticMR on either the MR-Sim or MR-Linac. SyntheticMR can generate inherently co-registered T1, T2, and PD quantitative maps along with synthetically generated weighted and inversion recovery images in under six minutes. This has the potential to replace current time-intensive sequences and complex registration techniques currently used in the radiation oncology workflow for more efficient biomarker-based adaptive radiation therapy, increasing the adoption of more specialized quantitative imaging biomarkers approaches⁴² at high temporal density. Some previously studied examples in the head and neck which could be adopted due to the time savings of SyntheticMR include apparent diffusion coefficient (ADC)⁴³,

dynamic contrast enhanced (DCE)⁴⁴, diffusion-weighted imaging (DWI)⁴⁵, and more emerging biomarkers such as T1-rho⁴⁶. Further, the geometric accuracy test was well within passing criteria providing sufficient confidence for radiation therapy setup, planning, and delivery.

Despite its promise, the current limitations of SyntheticMR include susceptibility to patient motion artifacts which would propagate to all generated maps, suppression of the blood signal causing black blood features, and ghosting artifacts due to flow sensitivity. Another simultaneous, multiparametric, technique which addresses some of these limitations and has been investigated by one prior group on the 1.5T MR-Linac⁹ is magnetic resonance fingerprinting, or MRF. This approach utilizes a series of dynamic scan acquisitions with each dynamic inheriting a pseudo-random set of acquisition parameters, typically the TR, TE, and flip angle. This pseudo-random acquired series is then matched to a pre-computed dictionary of MRI signal generation and fit to the most similar trajectory given the type of pulse sequence used. In comparison to SyntheticMR, MRF can acquire data using either a spin-echo or gradient-echo based approach allowing it to encode diffusion⁴⁷ and other weightings important in adaptive radiation therapy for head and neck cancer. However, MRF requires large pre-computed dictionary creation which may add prohibitive computational requirements. Further, MRF is only commercially available on Siemens MRI scanners providing only simultaneous T1 and T2 quantification at the time of this writing limiting its immediate clinical translation in comparison to SyntheticMR which is commercially available on Siemens, GE, and Philips.

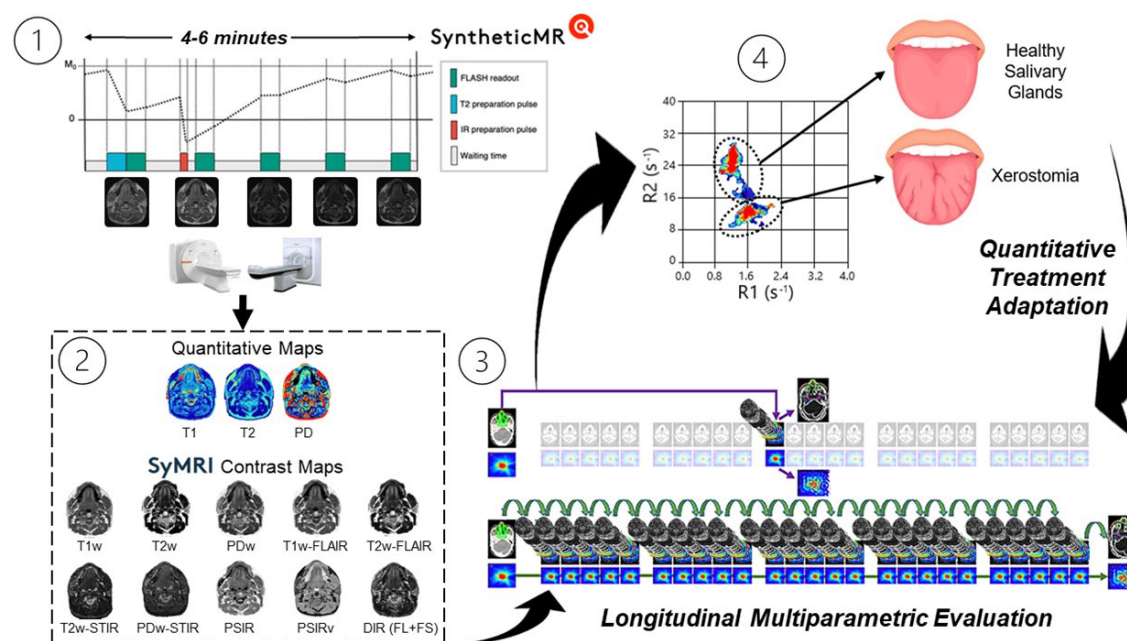


Figure 5: One potential application of SyntheticMR in the radiation oncology workflow to quantitatively adapt treatment based on detectable normal tissue damage in the salivary glands: 1) MRI acquisition overview, 2) generation of quantitative maps and subsequent synthetic contrast maps from SyMRI, 3) longitudinal acquisition schedule with high daily temporal resolution, and 4) subsequent evaluation of the deviations in the SyntheticMR maps. Note, the pulse sequence diagram (adapted from Fujita et al. 2024¹⁵) on the top left is for the 3D-QALAS sequence, not the 2D-MDME used in this study. Further, the figure on the bottom right is adapted from Heukelom and Fuller 2022⁴⁸.

The future applications of SyntheticMR in the general radiation oncology workflow is wide. Recent movements have suggested the transition to probabilistic target definition instead of the currently used uniform target definitions⁴⁹ which builds upon the ideas presented in dose painting⁵⁰. SyntheticMR has the potential to become a valuable asset in this space due to its multiparametric quantitative input at the voxel level which will help to inform probabilistic target definitions and optimal dose painting strategies. Techniques such as Bayesian and spatial statistics may also be employed upon SyntheticMR output to assess treatment response, identify sub-volume boost regions, and create more robust tumor control probability (TCP) and normal tissue complication probability (NTCP) models.

The multiparametric quantitative input at the voxel level may also be used as additional input channels for advanced image segmentation algorithms. This approach may be done manually using spatial statistics approaches, or automatically using deep learning techniques to identify optimal boundaries for each desired ROI in the three-dimensional quantitative space (T1 vs. T2 vs. PD). These boundaries may be created using large cohort studies of healthy volunteers and those with malignancies to generate consensus clusters for each desired ROI. Additional features from the synthetically generated contrast maps, such as radiomics, may also be included for improved performance²⁴. Similar research utilizing SyntheticMR to achieve these tasks in the brain for white matter, gray matter, and others has been successfully demonstrated and employed clinically as a product of SyntheticMR. Additionally, after these regions have been successfully determined and validated, they may be used to assess the error of clinical contours and quantify contour uncertainty in the presence of more homogeneous or heterogeneous ROIs.

5. Conclusion

SyntheticMR is a promising novel approach to consolidate the currently inhibitory time requirements for multiparametric MRI acquisition incorporating both anatomical scans and quantitative information. In this paper, we demonstrated the potential of SyntheticMR to enhance the radiation oncology workflow in the following ways: 1) achievement of multi-contrast anatomical information and quantification in a single scan acquisition time allowing for higher throughput or addition of more research sequences 2) superior simultaneous quantitative accuracy at higher spatial resolution compared to existing techniques, and 3) clinically acceptable repeatability, reproducibility, and spatial accuracy. These factors aligned with the high temporal resolution of the MR-Linac (i.e., 33 fractions for a head and neck cancer patient) will exponentially increase both the clinical and research efficiency of the MR-Linac inside the adaptive radiation therapy workflow as it is currently used allowing for more effective balancing of tumor control with reduction of normal tissue toxicity.

References




1. Shankar L, Montanera W. Computed Tomography Versus Magnetic Resonance Imaging and Three-Dimensional Applications. *Medical Clinics of North America*. 1991;75(6):1355-1366. doi:10.1016/S0025-7125(16)30392-3




2. Raaymakers BW, Lagendijk JJW, Overweg J, et al. Integrating a 1.5 T MRI scanner with a 6 MV accelerator: proof of concept. *Phys Med Biol.* 2009;54(12):N229-N237. doi:10.1088/0031-9155/54/12/N01
3. Cashmore MT, McCann AJ, Wastling SJ, McGrath C, Thornton J, Hall MG. Clinical quantitative MRI and the need for metrology. *The British Journal of Radiology.* 2021;94(1120):20201215. doi:10.1259/bjr.20201215
4. Qu J, Pan B, Su T, et al. T1 and T2 mapping for identifying malignant lymph nodes in head and neck squamous cell carcinoma. *Cancer Imaging.* 2023;23(1):125. doi:10.1186/s40644-023-00648-6
5. Kim SE, Roberts JA, Kholmovski EG, Hitchcock Y, Anzai Y. T1 mapping for Head and Neck Cancer Patients undergoing Chemoradiotherapy: Feasibility of 3D Stack of Star Imaging. *Magnetic Resonance Imaging.* 2024;112:38-46. doi:10.1016/j.mri.2024.04.005
6. Guerreiro F, Van Houdt PJ, Navest RJM, et al. Validation of quantitative magnetic resonance imaging techniques in head and neck healthy structures involved in the salivary and swallowing function: Accuracy and repeatability. *Physics and Imaging in Radiation Oncology.* 2024;31:100608. doi:10.1016/j.phro.2024.100608
7. Kooreman ES, Van Houdt PJ, Nowee ME, et al. Feasibility and accuracy of quantitative imaging on a 1.5 T MR-linear accelerator. *Radiotherapy and Oncology.* 2019;133:156-162. doi:10.1016/j.radonc.2019.01.011
8. Subashi E, LoCastro E, Apte A, Zelefsky MJ, Tyagi N. Quantitative Relaxometry for Target Localization and Response Assessment in Ultra-Hypofractionated MR-Guided Radiotherapy to the Prostate and DIL. *International Journal of Radiation Oncology*Biophysics*Physics.* 2022;114(3):S33. doi:10.1016/j.ijrobp.2022.07.390
9. Bruijnen T, Van Der Heide O, Intven MPW, et al. Technical feasibility of magnetic resonance fingerprinting on a 1.5T MRI-linac. *Phys Med Biol.* 2020;65(22):22NT01. doi:10.1088/1361-6560/abbb9d
10. Grimbergen G, Hackett SL, Van Ommen F, et al. Gating and intrafraction drift correction on a 1.5 T MR-Linac: Clinical dosimetric benefits for upper abdominal tumors. *Radiotherapy and Oncology.* 2023;189:109932. doi:10.1016/j.radonc.2023.109932
11. Warntjes JBM, Leinhard OD, West J, Lundberg P. Rapid magnetic resonance quantification on the brain: Optimization for clinical usage. *Magnetic Resonance in Med.* 2008;60(2):320-329. doi:10.1002/mrm.21635
12. Hagiwara A, Hori M, Cohen-Adad J, et al. Linearity, Bias, Intrascanner Repeatability, and Interscanner Reproducibility of Quantitative Multidynamic Multiecho Sequence for Rapid Simultaneous Relaxometry at 3 T: A Validation Study With a Standardized Phantom and Healthy Controls. *Invest Radiol.* 2019;54(1):39-47. doi:10.1097/RLI.0000000000000510
13. Hagiwara A, Warntjes M, Hori M, et al. SyMRI of the Brain: Rapid Quantification of Relaxation Rates and Proton Density, With Synthetic MRI, Automatic Brain Segmentation, and Myelin Measurement. *Invest Radiol.* 2017;52(10):647-657. doi:10.1097/RLI.0000000000000365







14. Kvernby S, Warntjes MJB, Haraldsson H, Carlhäll CJ, Engvall J, Ebbers T. Simultaneous three-dimensional myocardial T1 and T2 mapping in one breath hold with 3D-QALAS. *Journal of Cardiovascular Magnetic Resonance*. 2014;16(1):102. doi:10.1186/s12968-014-0102-0
15. Fujita S, Hagiwara A, Hori M, et al. Three-dimensional high-resolution simultaneous quantitative mapping of the whole brain with 3D-QALAS: An accuracy and repeatability study. *Magnetic Resonance Imaging*. 2019;63:235-243. doi:10.1016/j.mri.2019.08.031
16. Fujita S, Gagoski B, Hwang K, et al. Cross-vendor multiparametric mapping of the human brain using 3D-QALAS : A multicenter and multivendor study. *Magnetic Resonance in Med*. 2024;91(5):1863-1875. doi:10.1002/mrm.29939
17. Hwang K, Fujita S. Synthetic MR: Physical principles, clinical implementation, and new developments. *Medical Physics*. 2022;49(7):4861-4874. doi:10.1002/mp.15686
18. Xu S, Ma Z, Zhang J, et al. Quantitative assessment of preoperative brain development in pediatric congenital heart disease patients by synthetic MRI. *Insights Imaging*. 2024;15(1):166. doi:10.1186/s13244-024-01746-0
19. Zhang P, Yang J, Shu Y, et al. The value of synthetic MRI in detecting the brain changes and hearing impairment of children with sensorineural hearing loss. *Front Neurosci*. 2024;18:1365141. doi:10.3389/fnins.2024.1365141
20. Lin L, Chen Y, Dai Y, et al. Quantification of myelination in children with attention-deficit/hyperactivity disorder: a comparative assessment with synthetic MRI and DTI. *Eur Child Adolesc Psychiatry*. 2024;33(6):1935-1944. doi:10.1007/s00787-023-02297-3
21. Zhang L, Mai W, Mo X, et al. Quantitative evaluation of meniscus injury using synthetic magnetic resonance imaging. *BMC Musculoskelet Disord*. 2024;25(1):292. doi:10.1186/s12891-024-07375-4
22. Qu M, Feng W, Liu X, et al. Investigation of synthetic MRI with quantitative parameters for discriminating axillary lymph nodes status in invasive breast cancer. *European Journal of Radiology*. 2024;175:111452. doi:10.1016/j.ejrad.2024.111452
23. Chen Y, Meng T, Cao W, et al. Histogram analysis of MR quantitative parameters: are they correlated with prognostic factors in prostate cancer? *Abdom Radiol*. 2024;49(5):1534-1544. doi:10.1007/s00261-024-04227-6
24. Hwang KP, Elshafeey NA, Kotrotsou A, et al. A Radiomics Model Based on Synthetic MRI Acquisition for Predicting Neoadjuvant Systemic Treatment Response in Triple-Negative Breast Cancer. *Radiology: Imaging Cancer*. 2023;5(4):e230009. doi:10.1148/rycan.230009
25. Ljusberg A, Blystad I, Lundberg P, Adolfsson E, Tisell A. Radiation-dependent demyelination in normal appearing white matter in glioma patients, determined using quantitative magnetic resonance imaging. *Physics and Imaging in Radiation Oncology*. 2023;27:100451. doi:10.1016/j.phro.2023.100451

26. Zhang H, Hu L, Qin F, et al. Synthetic MRI and diffusion-weighted imaging for differentiating nasopharyngeal lymphoma from nasopharyngeal carcinoma: combination with morphological features. *British Journal of Radiology*. 2024;97(1159):1278-1285. doi:10.1093/bjr/tqae095
27. Konar AS, Paudyal R, Shah AD, et al. Qualitative and Quantitative Performance of Magnetic Resonance Image Compilation (MAGiC) Method: An Exploratory Analysis for Head and Neck Imaging. *Cancers*. 2022;14(15):3624. doi:10.3390/cancers14153624
28. Verkooijen HM, Kerkmeijer LGW, Fuller CD, et al. R-IDEAL: A Framework for Systematic Clinical Evaluation of Technical Innovations in Radiation Oncology. *Front Oncol*. 2017;7. doi:10.3389/fonc.2017.00059
29. Joint Head and Neck Radiotherapy-MRI Development Cooperative, Mohamed ASR, Abusaif A, et al. Prospective validation of diffusion-weighted MRI as a biomarker of tumor response and oncologic outcomes in head and neck cancer: Results from an observational biomarker pre-qualification study. Published online April 18, 2022. doi:10.1101/2022.04.18.22273782
30. Benedict SH, Yenice KM, Followill D, et al. Stereotactic body radiation therapy: The report of AAPM Task Group 101. *Medical Physics*. 2010;37(8):4078-4101. doi:10.1118/1.3438081
31. Vishwanath V, Jafarieh S, Rembielak A. The role of imaging in head and neck cancer: An overview of different imaging modalities in primary diagnosis and staging of the disease. *jcb*. 2020;12(5):512-518. doi:10.5114/jcb.2020.100386
32. Brahmbhatt S, Overfield CJ, Rhyner PA, Bhatt AA. Imaging of the Posttreatment Head and Neck: Expected Findings and Potential Complications. *Radiology: Imaging Cancer*. 2024;6(1):e230155. doi:10.1148/rycan.230155
33. Carr ME, Keenan KE, Rai R, Metcalfe P, Walker A, Holloway L. Determining the longitudinal accuracy and reproducibility of T₁ and T₂ in a 3T MRI scanner. *J Applied Clin Med Phys*. 2021;22(11):143-150. doi:10.1002/acm2.13432
34. Tijssen RHN, Philippens MEP, Paulson ES, et al. MRI commissioning of 1.5T MR-linac systems – a multi-institutional study. *Radiotherapy and Oncology*. 2019;132:114-120. doi:10.1016/j.radonc.2018.12.011
35. Fedorov A, Beichel R, Kalpathy-Cramer J, et al. 3D Slicer as an image computing platform for the Quantitative Imaging Network. *Magnetic Resonance Imaging*. 2012;30(9):1323-1341. doi:10.1016/j.mri.2012.05.001
36. Stupic KF, Ainslie M, Boss MA, et al. A standard system phantom for magnetic resonance imaging. *Magnetic Resonance in Med*. 2021;86(3):1194-1211. doi:10.1002/mrm.28779
37. Lang TA, Altman DG. Basic statistical reporting for articles published in Biomedical Journals: The “Statistical Analyses and Methods in the Published Literature” or the SAMPL Guidelines. *International Journal of Nursing Studies*. 2015;52(1):5-9. doi:10.1016/j.ijnurstu.2014.09.006
38. Bojorquez JZ, Bricq S, Acquitter C, Brunotte F, Walker PM, Lalande A. What are normal relaxation times of tissues at 3 T? *Magnetic Resonance Imaging*. 2017;35:69-80. doi:10.1016/j.mri.2016.08.021

39. Altman DG, Bland JM. Measurement in Medicine: The Analysis of Method Comparison Studies. *The Statistician*. 1983;32(3):307. doi:10.2307/2987937
40. Liu Y, Hayes DN, Nobel A, Marron JS. Statistical Significance of Clustering for High-Dimension, Low-Sample Size Data. *Journal of the American Statistical Association*. 2008;103(483):1281-1293. doi:10.1198/016214508000000454
41. Liao J, Saito N, Ozonoff A, Jara H, Steinberg M, Sakai O. Quantitative MRI analysis of salivary glands in sickle cell disease. *Dentomaxillofac Radiol*. 2012;41(8):630-636. doi:10.1259/dmfr/31672000
42. Van Houdt PJ, Saeed H, Thorwarth D, et al. Integration of quantitative imaging biomarkers in clinical trials for MR-guided radiotherapy: Conceptual guidance for multicentre studies from the MR-Linac Consortium Imaging Biomarker Working Group. *European Journal of Cancer*. 2021;153:64-71. doi:10.1016/j.ejca.2021.04.041
43. El-Habashy DM, Wahid KA, He R, et al. Longitudinal diffusion and volumetric kinetics of head and neck cancer magnetic resonance on a 1.5 T MR-linear accelerator hybrid system: A prospective R-IDEAL stage 2a imaging biomarker characterization/pre-qualification study. *Clinical and Translational Radiation Oncology*. 2023;42:100666. doi:10.1016/j.ctro.2023.100666
44. Khamis Y, Mohamed AS, Abobakr M, et al. Dynamic Contrast Enhanced MRI as a Biomarker of Tumor Response and Oncologic Outcomes in Head and Neck Cancer: Results of a Single Institution Prospective Imaging Study. *International Journal of Radiation Oncology*Biophysics*. 2023;117(2):e677-e678. doi:10.1016/j.ijrobp.2023.06.2134
45. McDonald BA, Salzillo T, Mulder S, et al. Prospective evaluation of in vivo and phantom repeatability and reproducibility of diffusion-weighted MRI sequences on 1.5 T MRI-linear accelerator (MR-Linac) and MR simulator devices for head and neck cancers. *Radiotherapy and Oncology*. 2023;185:109717. doi:10.1016/j.radonc.2023.109717
46. Kooreman ES, Tanaka M, Ter Beek LC, et al. T1p for Radiotherapy Treatment Response Monitoring in Rectal Cancer Patients: A Pilot Study. *JCM*. 2022;11(7):1998. doi:10.3390/jcm11071998
47. Afzali M, Mueller L, Sakaie K, et al. MR Fingerprinting with b-Tensor Encoding for Simultaneous Quantification of Relaxation and Diffusion in a Single Scan. *Magnetic Resonance in Med*. 2022;88(5):2043-2057. doi:10.1002/mrm.29352
48. Heukelom J, Fuller CD. Head and Neck Cancer Adaptive Radiation Therapy (ART): Conceptual Considerations for the Informed Clinician. *Seminars in Radiation Oncology*. 2019;29(3):258-273. doi:10.1016/j.semradonc.2019.02.008
49. Ferjančič P, Van Der Heide UA, Ménard C, Jeraj R. Probabilistic target definition and planning in patients with prostate cancer. *Phys Med Biol*. 2021;66(21):215011. doi:10.1088/1361-6560/ac2f8a
50. Fredén E, Tilly D, Ahnesjö A. Adaptive dose painting for prostate cancer. *Front Oncol*. 2022;12:973067. doi:10.3389/fonc.2022.973067







Price: \$200.00
 Item Number: 2000
 Item Cap: 1.0000
 Item Size: 2000.0000



1.
 2.
 3.
 4.
 5.
 6.
 7.
 8.
 9.
 10.
 11.
 12.
 13.
 14.
 15.
 16.
 17.
 18.
 19.
 20.
 21.
 22.
 23.
 24.
 25.
 26.
 27.
 28.
 29.
 30.
 31.
 32.
 33.
 34.
 35.
 36.
 37.
 38.
 39.
 40.
 41.
 42.
 43.
 44.
 45.
 46.
 47.
 48.
 49.
 50.
 51.
 52.
 53.
 54.
 55.
 56.
 57.
 58.
 59.
 60.
 61.
 62.
 63.
 64.
 65.
 66.
 67.
 68.
 69.
 70.
 71.
 72.
 73.
 74.
 75.
 76.
 77.
 78.
 79.
 80.
 81.
 82.
 83.
 84.
 85.
 86.
 87.
 88.
 89.
 90.
 91.
 92.
 93.
 94.
 95.
 96.
 97.
 98.
 99.
 100.



100% (100/100)
 100% (100/100)
 100% (100/100)
 100% (100/100)

```

root@kali:~# cat /etc/passwd | grep root
root:x:0:0:root:/root:/bin/bash
root:x:1:1:daemon:/usr/sbin:/usr/sbin/nologin
root:x:2:2:bin:/usr/sbin:/usr/sbin/nologin

```



1. **1.1** **1.1**
 1.2 **1.2**
 1.3 **1.3**
 1.4 **1.4**
 1.5 **1.5**
 1.6 **1.6**
 1.7 **1.7**
 1.8 **1.8**
 1.9 **1.9**
 1.10 **1.10**
 1.11 **1.11**
 1.12 **1.12**
 1.13 **1.13**
 1.14 **1.14**
 1.15 **1.15**
 1.16 **1.16**
 1.17 **1.17**
 1.18 **1.18**
 1.19 **1.19**
 1.20 **1.20**
 1.21 **1.21**
 1.22 **1.22**
 1.23 **1.23**
 1.24 **1.24**
 1.25 **1.25**
 1.26 **1.26**
 1.27 **1.27**
 1.28 **1.28**
 1.29 **1.29**
 1.30 **1.30**
 1.31 **1.31**
 1.32 **1.32**
 1.33 **1.33**
 1.34 **1.34**
 1.35 **1.35**
 1.36 **1.36**
 1.37 **1.37**
 1.38 **1.38**
 1.39 **1.39**
 1.40 **1.40**
 1.41 **1.41**
 1.42 **1.42**
 1.43 **1.43**
 1.44 **1.44**
 1.45 **1.45**
 1.46 **1.46**
 1.47 **1.47**
 1.48 **1.48**
 1.49 **1.49**
 1.50 **1.50**
 1.51 **1.51**
 1.52 **1.52**
 1.53 **1.53**
 1.54 **1.54**
 1.55 **1.55**
 1.56 **1.56**
 1.57 **1.57**
 1.58 **1.58**
 1.59 **1.59**
 1.60 **1.60**
 1.61 **1.61**
 1.62 **1.62**
 1.63 **1.63**
 1.64 **1.64**
 1.65 **1.65**
 1.66 **1.66**
 1.67 **1.67**
 1.68 **1.68**
 1.69 **1.69**
 1.70 **1.70**
 1.71 **1.71**
 1.72 **1.72**
 1.73 **1.73**
 1.74 **1.74**
 1.75 **1.75**
 1.76 **1.76**
 1.77 **1.77**
 1.78 **1.78**
 1.79 **1.79**
 1.80 **1.80**
 1.81 **1.81**
 1.82 **1.82**
 1.83 **1.83**
 1.84 **1.84**
 1.85 **1.85**
 1.86 **1.86**
 1.87 **1.87**
 1.88 **1.88**
 1.89 **1.89**
 1.90 **1.90**
 1.91 **1.91**
 1.92 **1.92**
 1.93 **1.93**
 1.94 **1.94**
 1.95 **1.95**
 1.96 **1.96**
 1.97 **1.97**
 1.98 **1.98**
 1.99 **1.99**
 2.00 **2.00**
 2.01 **2.01**
 2.02 **2.02**
 2.03 **2.03**
 2.04 **2.04**
 2.05 **2.05**
 2.06 **2.06**
 2.07 **2.07**
 2.08 **2.08**
 2.09 **2.09**
 2.10 **2.10**
 2.11 **2.11**
 2.12 **2.12**
 2.13 **2.13**
 2.14 **2.14**
 2.15 **2.15**
 2.16 **2.16**
 2.17 **2.17**
 2.18 **2.18**
 2.19 **2.19**
 2.20 **2.20**
 2.21 **2.21**
 2.22 **2.22**
 2.23 **2.23**
 2.24 **2.24**
 2.25 **2.25**
 2.26 **2.26**
 2.27 **2.27**
 2.28 **2.28**
 2.29 **2.29**
 2.30 **2.30**
 2.31 **2.31**
 2.32 **2.32**
 2.33 **2.33**
 2.34 **2.34**
 2.35 **2.35**
 2.36 **2.36**
 2.37 **2.37**
 2.38 **2.38**
 2.39 **2.39**
 2.40 **2.40**
 2.41 **2.41**
 2.42 **2.42**
 2.43 **2.43**
 2.44 **2.44**
 2.45 **2.45**
 2.46 **2.46**
 2.47 **2.47**
 2.48 **2.48**
 2.49 **2.49**
 2.50 **2.50**
 2.51 **2.51**
 2.52 **2.52**
 2.53 **2.53**
 2.54 **2.54**
 2.55 **2.55**
 2.56 **2.56**
 2.57 **2.57**
 2.58 **2.58**
 2.59 **2.59**
 2.60 **2.60**
 2.61 **2.61**
 2.62 **2.62**
 2.63 **2.63**
 2.64 **2.64**
 2.65 **2.65**
 2.66 **2.66**
 2.67 **2.67**
 2.68 **2.68**
 2.69 **2.69**
 2.70 **2.70**
 2.71 **2.71**
 2.72 **2.72**
 2.73 **2.73**
 2.74 **2.74**
 2.75 **2.75**
 2.76 **2.76**
 2.77 **2.77**
 2.78 **2.78**
 2.79 **2.79**
 2.80 **2.80**
 2.81 **2.81**
 2.82 **2.82**
 2.83 **2.83**
 2.84 **2.84**
 2.85 **2.85**
 2.86 **2.86**
 2.87 **2.87**
 2.88 **2.88**
 2.89 **2.89**
 2.90 **2.90**
 2.91 **2.91**
 2.92 **2.92**
 2.93 **2.93**
 2.94 **2.94**
 2.95 **2.95**
 2.96 **2.96**
 2.97 **2.97**
 2.98 **2.98**
 2.99 **2.99**
 3.00 **3.00**
 3.01 **3.01**
 3.02 **3.02**
 3.03 **3.03**
 3.04 **3.04**
 3.05 **3.05**
 3.06 **3.06**
 3.07 **3.07**
 3.08 **3.08**
 3.09 **3.09**
 3.10 **3.10**
 3.11 **3.11**
 3.12 **3.12**
 3.13 **3.13**
 3.14 **3.14**
 3.15 **3.15**
 3.16 **3.16**

[illegible]

1992-1993: 1st year
 1994-1995: 2nd year
 1996-1997: 3rd year
 1998-1999: 4th year

1990 1991 1992
 1993 1994 1995 1996 1997
 1998 1999 2000 2001 2002
 2003 2004 2005 2006 2007 2008 2009 2010 2011 2012 2013 2014 2015 2016 2017 2018 2019 2020 2021 2022 2023 2024 2025 2026 2027 2028 2029 2030 2031 2032 2033 2034 2035 2036 2037 2038 2039 2040 2041 2042 2043 2044 2045 2046 2047 2048 2049 2050 2051 2052 2053 2054 2055 2056 2057 2058 2059 2060 2061 2062 2063 2064 2065 2066 2067 2068 2069 2070 2071 2072 2073 2074 2075 2076 2077 2078 2079 2080 2081 2082 2083 2084 2085 2086 2087 2088 2089 2090 2091 2092 2093 2094 2095 2096 2097 2098 2099 2100 2101 2102 2103 2104 2105 2106 2107 2108 2109 2110 2111 2112 2113 2114 2115 2116 2117 2118 2119 2120 2121 2122 2123 2124 2125 2126 2127 2128 2129 2130 2131 2132 2133 2134 2135 2136 2137 2138 2139 2140 2141 2142 2143 2144 2145 2146 2147 2148 2149 2150 2151 2152 2153 2154 2155 2156 2157 2158 2159 2160 2161 2162 2163 2164 2165 2166 2167 2168 2169 2170 2171 2172 2173 2174 2175 2176 2177 2178 2179 2180 2181 2182 2183 2184 2185 2186 2187 2188 2189 2190 2191 2192 2193 2194 2195 2196 2197 2198 2199 2200 2201 2202 2203 2204 2205 2206 2207 2208 2209 2210 2211 2212 2213 2214 2215 2216 2217 2218 2219 2220 2221 2222 2223 2224 2225 2226 2227 2228 2229 2230 2231 2232 2233 2234 2235 2236 2237 2238 2239 2240 2241 2242 2243 2244 2245 2246 2247 2248 2249 2250 2251 2252 2253 2254 2255 2256 2257 2258 2259 2260 2261 2262 2263 2264 2265 2266 2267 2268 2269 2270 2271 2272 2273 2274 2275 2276 2277 2278 2279 2280 2281 2282 2283 2284 2285 2286 2287 2288 2289 2290 2291 2292 2293 2294 2295 2296 2297 2298 2299 2300 2301 2302 2303 2304 2305 2306 2307 2308 2309 2310 2311 2312 2313 2314 2315 2316 2317 2318 2319 2320 2321 2322 2323 2324 2325 2326 2327 2328 2329 2330 2331 2332 2333 2334 2335 2336 2337 2338 2339 2340 2341 2342 2343 2344 2345 2346 2347 2348 2349 2350 2351 2352 2353 2354 2355 2356 2357 2358 2359 2360 2361 2362 2363 2364 2365 2366 2367 2368 2369 2370 2371 2372 2373 2374 2375 2376 2377 2378 2379 2380 2381 2382 2383 2384 2385 2386 2387 2388 2389 2390 2391 2392 2393 2394 2395 2396 2397 2398 2399 2400 2401 2402 2403 2404 2405 2406 2407 2408 2409 2410 2411 2412 2413 2414 2415 2416 2417 2418 2419 2420 2421 2422 2423 2424 2425 2426 2427 2428 2429 2430 2431 2432 2433 2434 2435 2436 2437 2438 2439 2440 2441 2442 2443 2444 2445 2446 2447 2448 2449 2450 2451 2452 2453 2454 2455 2456 2457 2458 2459 2460 2461 2462 2463 2464 2465 2466 2467 2468 2469 2470 2471 2472 2473 2474 2475 2476 2477 2478 2479 2480 2481 2482 2483 2484 2485 2486 2487 2488 2489 2490 2491 2492 2493 2494 2495 2496 2497 2498 2499 2500 2501 2502 2503 2504 2505 2506 2507 2508 2509 2510 2511 2512 2513 2514 2515 2516 2517 2518 2519 2520 2521 2522 2523 2524 2525 2526 2527 2528 2529 2530 2531 2532 2533 2534 2535 2536 2537 2538 2539 2540 2541 2542 2543 2544 2545 2546 2547 2548 2549 2550 2551 2552 2553 2554 2555 2556 2557 2558 2559 2560 2561 2562 2563 2564 2565 2566 2567 2568 2569 2570 2571 2572 2573 2574 2575 2576 2577 2578 2579 2580 2581 2582 2583 2584 2585 2586 2587 2588 2589 2590 2591 2592 2593 2594 2595 2596 2597 2598 2599 2600 2601 2602 2603 2604 2605 2606 2607 2608 2609 2610 2611 2612 2613 2614 2615 2616 2617 2618 2619 2620 2621 2622 2623 2624 2625 2626 2627 2628 2629 2630 2631 2632 2633 2634 2635 2636 2637 2638 2639 2640 2641 2642 2643 2644 2645 2646 2647 2648 2649 2650 2651 2652 2653 2654 2655 2656 2657 2658 2659 2660 2661 2662 2663 2664 2665 2666 2667 2668 2669 2670 2671 2672 2673 2674 2675 2676 2677 2678 2679 2680 2681 2682 2683 2684 2685 2686 2687 2688 2689 2690 2691 2692 2693 2694 2695 2696 2697 2698 2699 2700 2701 2702 2703 2704 2705 2706 2707 2708 2709 2710 2711 2712 2713 2714 2715 2716 2717 2718 2719 2720 2721 2722 2723 2724 2725 2726 2727 2728 2729 2730 2731 2732 2733 2734 2735 2736 2737 2738 2739 2740 2741 2742 2743 2744 2745 2746 2747 2748 2749 2750 2751 2752 2753 2754 2755 2756 2757 2758 2759 2760 2761 2762 2763 2764 2765 2766 2767 2768 2769 2770 2771 2772 2773 2774 2775 2776 2777 2778 2779 2780 2781 2782 2783 2784 2785 2786 2787 2788 2789 2790 2791 2792 2793 2794 2795 2796 2797 2798 2799 2800 2801 2802 2803 2804 2805



11
 12
 13
 14
 15
 16
 17
 18
 19
 20
 21
 22
 23
 24
 25
 26
 27
 28
 29
 30
 31
 32
 33
 34
 35
 36
 37
 38
 39
 40
 41
 42
 43
 44
 45
 46
 47
 48
 49
 50
 51
 52
 53
 54
 55
 56
 57
 58
 59
 60
 61
 62
 63
 64
 65
 66
 67
 68
 69
 70
 71
 72
 73
 74
 75
 76
 77
 78
 79
 80
 81
 82
 83
 84
 85
 86
 87
 88
 89
 90
 91
 92
 93
 94
 95
 96
 97
 98
 99
 100
 101
 102
 103
 104
 105
 106
 107
 108
 109
 110
 111
 112
 113
 114
 115
 116
 117
 118
 119
 120
 121
 122
 123
 124
 125
 126
 127
 128
 129
 130
 131
 132
 133
 134
 135
 136
 137
 138
 139
 140
 141
 142
 143
 144
 145
 146
 147
 148
 149
 150
 151
 152
 153
 154
 155
 156
 157
 158
 159
 160
 161
 162
 163
 164
 165
 166
 167
 168
 169
 170
 171
 172
 173
 174
 175
 176
 177
 178
 179
 180
 181
 182
 183
 184
 185
 186
 187
 188
 189
 190
 191
 192
 193
 194
 195
 196
 197
 198
 199
 200
 201
 202
 203
 204
 205
 206
 207
 208
 209
 210
 211
 212
 213
 214
 215
 216
 217
 218
 219
 220
 221
 222
 223
 224
 225
 226
 227
 228
 229
 230
 231
 232
 233
 234
 235
 236
 237
 238
 239
 240
 241
 242
 243
 244
 245
 246
 247
 248
 249
 250
 251
 252
 253
 254
 255
 256
 257
 258
 259
 260
 261
 262
 263
 264
 265
 266
 267
 268
 269
 270
 271
 272
 273
 274
 275
 276
 277
 278
 279
 280
 281
 282
 283
 284
 285
 286
 287
 288
 289
 290
 291
 292
 293
 294
 295
 296
 297
 298
 299
 300
 301
 302
 303
 304
 305
 306
 307
 308
 309
 310
 311
 312
 313
 314
 315
 316
 317
 318
 319
 320
 321
 322
 323
 324
 325
 326
 327
 328
 329
 330
 331
 332
 333
 334
 335
 336
 337
 338
 339
 340
 341
 342
 343
 344
 345
 346
 347
 348
 349
 350
 351
 352
 353
 354
 355
 356
 357
 358
 359
 360
 361
 362
 363
 364
 365
 366
 367
 368
 369
 370
 371
 372
 373
 374
 375
 376
 377
 378
 379
 380
 381
 382
 383
 384
 385
 386
 387
 388
 389
 390
 391
 392
 393
 394
 395
 396
 397
 398
 399
 400
 401
 402
 403
 404
 405
 406
 407
 408
 409
 410
 411
 412
 413
 414
 415
 416
 417
 418
 419
 420
 421
 422
 423
 424
 425
 426
 427
 428
 429
 430
 431
 432
 433
 434
 435
 436
 437
 438
 439
 440
 441
 442
 443
 444
 445
 446
 447
 448
 449
 450
 451
 452
 453
 454
 455
 456
 457
 458
 459
 460
 461
 462
 463
 464
 465
 466
 467
 468
 469
 470
 471
 472
 473
 474
 475
 476
 477
 478
 479
 480
 481
 482
 483
 484
 485
 486
 487
 488
 489
 490
 491
 492
 493
 494
 495
 496
 497
 498
 499
 500
 501
 502
 503
 504
 505
 506
 507
 508
 509
 510
 511
 512
 513
 514
 515
 516
 517
 518
 519
 520
 521
 522
 523
 524
 525
 526
 527
 528
 529
 530
 531
 532
 533



NAME: [REDACTED]
DOB: [REDACTED] **SSN:** [REDACTED]
ADDRESS: [REDACTED]
CITY: [REDACTED] **STATE:** [REDACTED] **ZIP:** [REDACTED]

100

[illegible]

