

Seasonal and daily variation in indoor light and temperature associate with sleep disturbance in dementia: Supplementary material

Anne C. Skeldon^{1,2,†}, Thalia Rodriguez Garcia^{1,2,3,†}, Centre for Care Research & Technology¹,
Eyal Sorek^{1,4}, Chloe Walsh^{1,4}, Derk-Jan Dijk^{1,3}

¹ School of Mathematics & Physics, Faculty of Engineering and Physical Sciences,
University of Surrey, Guildford, UK

² UK Dementia Research Institute, Care Research & Technology Centre,
Imperial College London, London and the University of Surrey, Guildford, UK

³ Surrey Sleep Research Centre, School of Biosciences, Faculty of Health and Medical Sciences,
University of Surrey, Guildford, UK

⁴ Department of Brain Sciences, Imperial College London, UK

† These authors contributed equally to the paper

Contents

- S1 Demographics 4
- S2 Definitions 5
- S3 Further figures 9
- S4 Tables summarising statistical results 12
- S5 Seasonal desynchrony 16

List of Figures

S1	Derivation of in-bed and sleep metrics from the bedmat. Graphical depiction of the process for defining metrics from the Withing’s sleep analyser (WSA) bedmat. The top panel illustrates the nature of the minute-to-minute data streamed from the bedmat. The lower panel describes how the minute-to-minute data is used to define in-bed and sleep periods and associated metrics.	5
S2	Between and within participant variation in indoor light and temperature environment, bed occupancy, respiratory rate and heart rate. Box plots for each participant showing the between and within participant variation in a few example metrics that quantify aspects of the indoor daytime light environment, the nighttime temperature environment, time in bed, respiratory rate and heart rate.	9
S3	Seasonal variation of in-bed duration, timing and fragmentation, physiology. The data shown are the Least Squares (LS) means from a linear mixed effect model which considers the seasonal variation for each measure controlling for gender, age and diagnosis with participant as a random effect (see Supplementary Table S5). Eight of the 25 measures are also shown in the Fig. 3 of the main text. All measures are included here for ease of visual comparison.	10
S4	Individual variation in total time in-bed. Time courses of the total time in-bed for each participants. Each data point is a single day. The magenta lines show the two-month moving averages.	11
S5	Desynchrony due to a maladaptive light environment? a) Raster plot for the heart rate for participant “seasonal”, replicated from Fig. 1 (b). Recording of heart rate during sleep for one night showing how the heart rate dips to a minimum. Superimposed on the raw data is a 60 minute moving average, with the circular marker indicating the minimum. (c) Mean daily light levels in the lounge for participant “seasonal”. (d) Raster plots of sleep predictions. In the left hand panel, it is assumed that light is not gated by sleep. In the right hand panel, it is assumed that the measured light is gated by sleep.	17

List of Tables

S1	Participant demographics.	4
S2	Daily and seasonal variation of the light and temperature environment. Results of a linear fixed effect model for average hourly light (log lux) and temperature (°C) for the fixed effects of hour of the day, two-month period, room and home. Hour, two-month period, room and home were all entered as categorical variables.	12
S3	Seasonal variation of the light and temperature environment. Results of a linear mixed effect model for various daily indoor light and temperature measures with the fixed effect of two-month period and the random effect of home.	12
S4	Descriptive statistics for the measures of sleep behaviour and physiology and the light and temperature environment Descriptive statistics describing the distribution of the $n = 70$ participant mean values for the 25 different measures of sleep behaviour and physiology and 4 measures of the light and temperature environment. The intraclass correlation coefficient for each measure is also included. For all measures, the reported mean is the mean of the participant mean values, i.e. from the approximately 26,000 days of data, the individual participant mean values were first calculated. Then the mean of the participant values was found.	13
S5	Seasonal effects on the duration, timing and fragmentation of bed occupancy and physiology. Results from a linear mixed effect model for the seasonal variation of the 25 measures of bed occupancy, physiology and a marker of the biological clock controlling for gender, age and diagnosis. One of the participant's did not have a diagnosis, so only 69 of the 70 participants were included in this analysis.	14
S6	Effects of light, temperature and time-in-study on the duration, timing and fragmentation of bed occupancy and on physiology. Linear mixed effect model results for the 25 measures of bed occupancy and physiology, extending the model reported in Table S5 to include environmental variables. Only the results for the additional variables (hours of bright light, mean nocturnal temperature, temperature amplitude and time-in-study) are shown. All other effects are similar to those reported in Supplementary Table S5). One of the participant's did not have a diagnosis, so only 69 of the 70 participants were included in this analysis.	15

S1 Demographics

	Number of participants	Age (+/-SD) (y)	MMSE (+/-SD)	Total NPI score (+/-SD)	NPI sleep score (+/-SD)	ADAS Cog (+/-SD)	Collection period (+/-SD) (d)	Days of data (+/-SD) (d)
All	70	79 (+/-9)	22 (+/-6)	12 (+/-10)	1.3 (+/-2.4)	36 (+/-16)	464 (+/-169)	379 (+/-149)
Men	44	78 (+/-9)	23 (+/-5)	11 (+/-10)	1.0 (+/-2.0)	37 (+/-16)	480 (+/-178)	393 (+/-154)
Women	26	81 (+/-9)	20 (+/-8)	13 (+/-10)	1.8 (+/-2.8)	33 (+/-15)	435 (+/-153)	355 (+/-139)
Alzheimer's diagnosis	48	80 (+/-8)	21 (+/-7)	11 (+/-10)	0.9 (+/-2.1)	38 (+/-14)	447 (+/-157)	368 (+/-135)
Other diagnosis	21	78 (+/-11)	22 (+/-5)	14 (+/-11)	2.0 (+/-2.8)	30 (+/-17)	511 (+/-191)	410 (+/-179)

Table S1: Participant demographics.

S2 Definitions

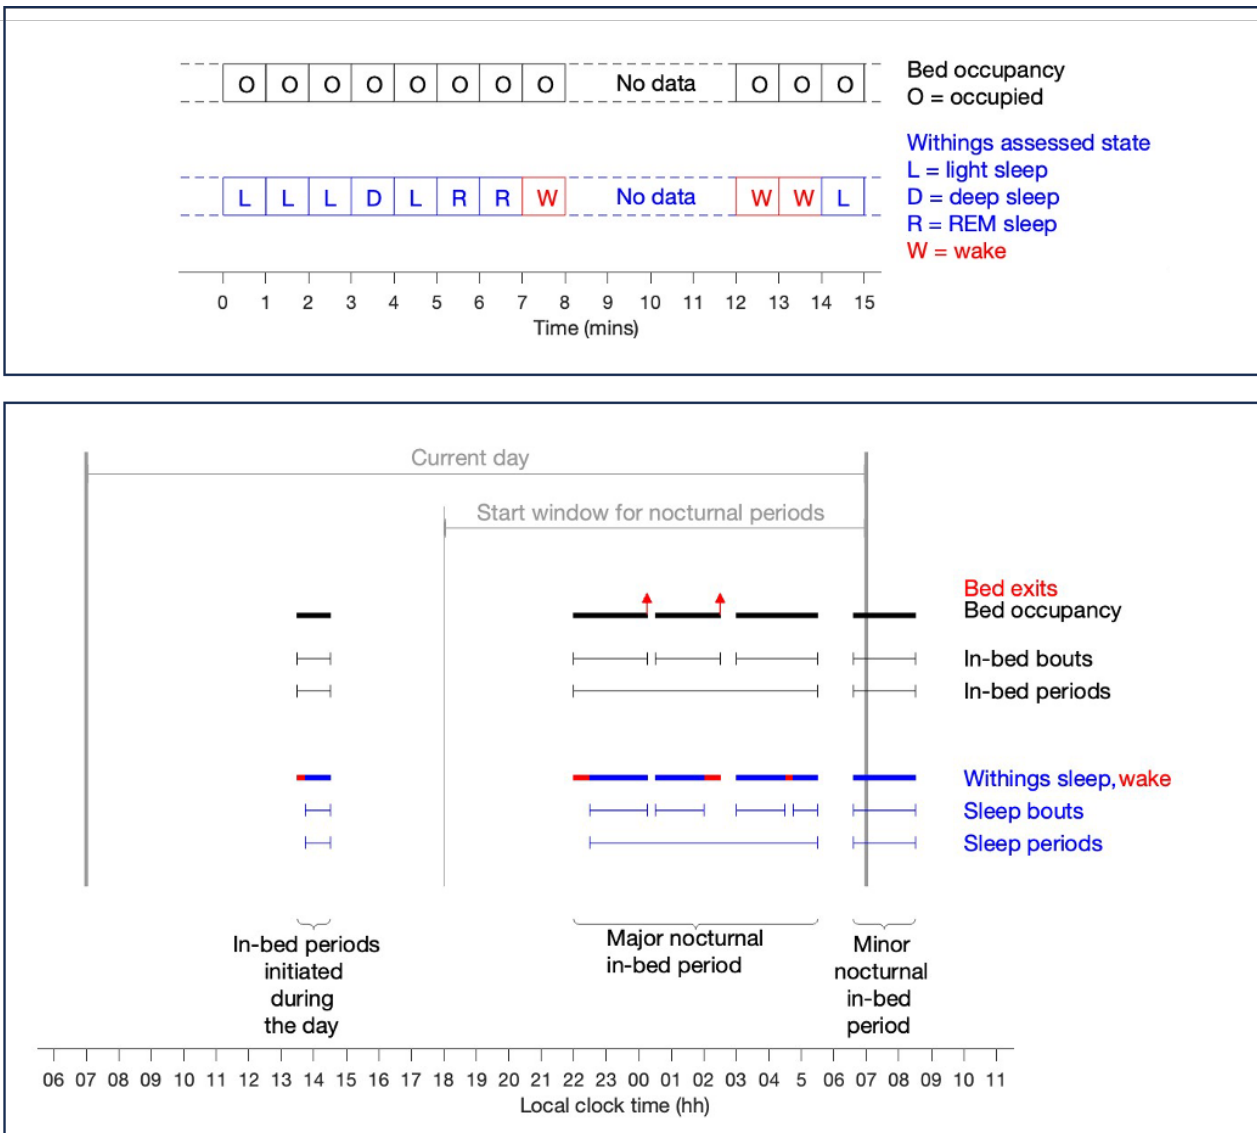


Figure S1: **Derivation of in-bed and sleep metrics from the bedmat.** Graphical depiction of the process for defining metrics from the Withings's sleep analyser (WSA) bedmat. The top panel illustrates the nature of the minute-to-minute data streamed from the bedmat. The lower panel describes how the minute-to-minute data is used to define in-bed and sleep periods and associated metrics.

Definitions

Total time in-bed (h) Total time that the Withings sleep analyser (WSA) registers that someone is in bed between 07:00 and 07:00.

In-bed bout A contiguous sequence of minutes in which the WSA registers that an individual is in bed. An in-bed bout has a start time, an end time and a duration (h).

Out-of-bed bouts An unbroken period of time in which the WSA registers no information.

Sleep bout A contiguous sequence of minutes in which the WSA registers that an individual is in one of deep, light or REM sleep. A sleep bout has a start time, an end time and a duration (h).

In-bed period A sequential group of in-bed bouts where the gap between successive in-bed bouts is less than one hour.

Sleep period A sequential group of sleep bouts where the gap between successive sleep bouts is less than one hour.

Nocturnal in-bed period An in-bed period where the start time of the first in-bed bout is after 18:00 and before 07:00 and at least 2 minutes are recorded as sleep.

Nocturnal sleep period A sleep period where the start time of the first sleep bout is after 18:00 and before 07:00 and the period is at least 2 minutes long.

Major nocturnal in-bed period The longest nocturnal in-bed period.

Major nocturnal sleep period The longest nocturnal sleep period.

Minor nocturnal in-bed periods All nocturnal in-bed periods other than the major nocturnal in-bed period.

Minor nocturnal sleep periods All nocturnal sleep periods other than the major nocturnal sleep period.

Current day The day leading up to the nocturnal in-bed period. For daily measures (e.g. the total time in-bed, the current day starts at 07:00.

Definitions related to in-bed periods initiated during the day

In-bed period initiated during the day An in-bed period with the start time of the first in-bed bout in the period after 07:00 and before 18:00 and at least 2 minutes are recorded as sleep.

Sleep period initiated during the day A sleep period with the start time of the first in-bed bout in the period after 07:00 and before 18:00 and the period is at least 2 minutes long.

Total duration of in-bed periods initiated during the day on the current day (h) The sum of the durations of all the in-bed periods that start during the day on the current day.

Definitions related to the major nocturnal period

Duration of the major nocturnal in-bed period (h) The period of time from the start of the major nocturnal in-bed period to the end of the major nocturnal in-bed period.

Onset time of the major nocturnal in-bed period The start time of the major nocturnal in-bed period.

Offset time of the major nocturnal time-in-bed period The end time of the major nocturnal in-bed period.

Definitions related to fragmentation

Number of bed exits Number of out-of-bed bouts during the major nocturnal time-in-bed period.

Bed exit rate (exits/h) Number of 'bed exits' / Major nocturnal in-bed period duration.

Median duration of bed exits (h) The median duration of out-of-bed bouts during the major nocturnal in-bed period.

Median duration of sleep bouts (h) The median duration of sleep bouts during the major nocturnal in-bed period.

Median duration of wake bouts (h) The median duration of wake bouts during the major nocturnal in-bed period.

Wake after sleep onset (h) The sum of the WSA wake state duration and the out-of-bed duration during the major nocturnal sleep period.

Sleep efficiency (%) $100 \times$ The nocturnal sleep duration / duration of the major nocturnal in-bed period.

Definitions related to physiology

Mean breathing rate (breaths/min) Mean breathing rate during the major nocturnal sleep period for minutes that the WSA registers that an individual is asleep.

Mean heart rate (beats/min) Mean heart rate recorded during the major nocturnal sleep period for minutes that the WSA registers than an individual is asleep.

Std dev. heart rate (beats/min) Standard deviation of the heart rate values recorded during the major nocturnal sleep period for minutes that the WSA registers than an individual is asleep.

Definitions related to the environment

Mean light intensity (lux) The mean light intensity recorded by the multi-sensor between 07:00 on the current day and 07:00 on the next day.

Geometric mean light intensity (lux) The geometric mean light intensity recorded by the multi-sensor between 07:00 on the current day and 07:00 on the next day.

Hours of bright light (h) The amount of time that the multi-sensor records light levels of 500 or more lux on the current day.

Mean daily temperature (°C) The mean temperature recorded by the multi-sensor between 07:00 on the current day and 07:00 on the next day.

Maximum daily temperature (°C) The maximum temperature recorded by the multi-sensor between 07:00 on the current day and 07:00 on the next day.

Minimum daily temperature (°C) The minimum temperature recorded by the multi-sensor between 07:00 on the current day and 07:00 on the next day.

Mean nocturnal temperature (°C) The mean temperature recorded by the multi-sensor during the major nocturnal in-bed period.

Temperature amplitude (°C) The difference between the maximum and minimum value of the temperature on each 24-hour period from 07:00 on the current day to 07:00 on the next day.

S3 Further figures

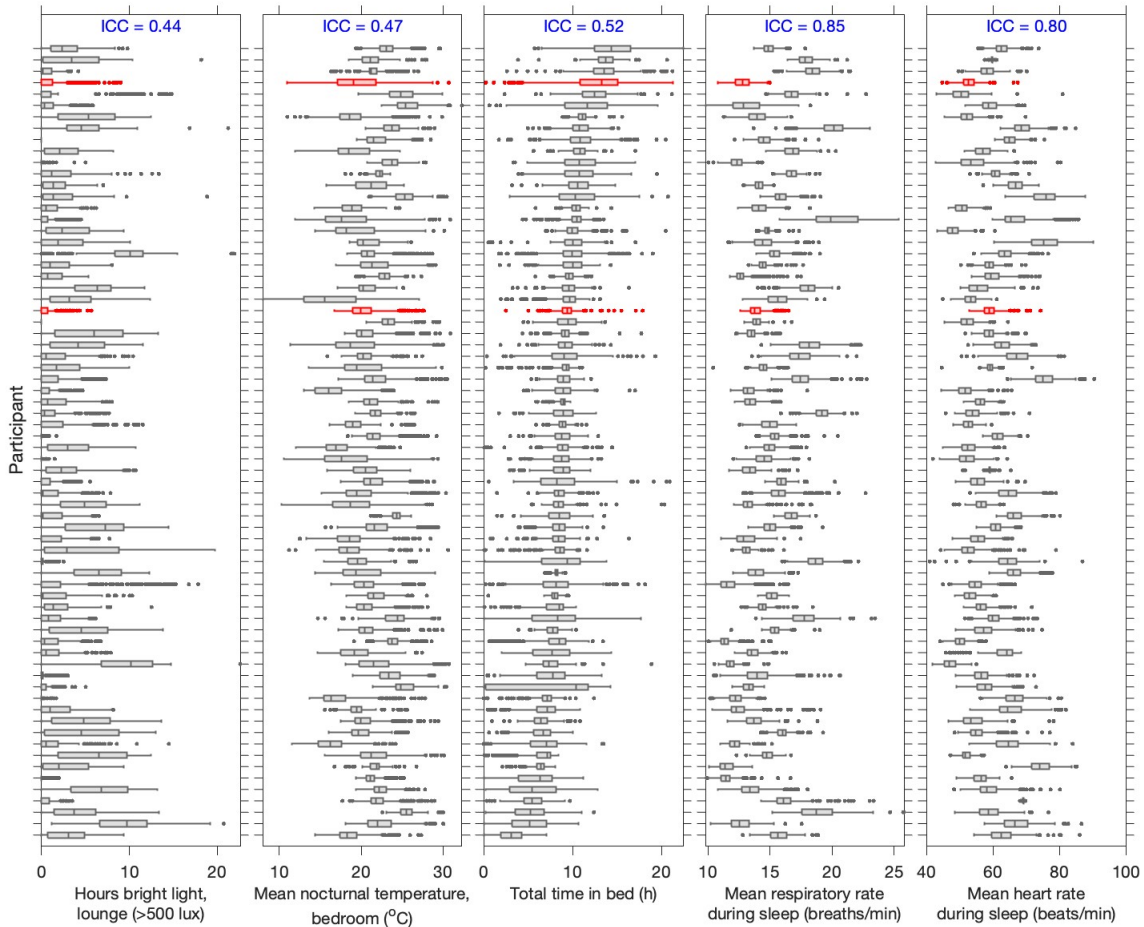


Figure S2: **Between and within participant variation in indoor light and temperature environment, bed occupancy, respiratory rate and heart rate.** Box plots for each participant showing the between and within participant variation in a few example metrics that quantify aspects of the indoor daytime light environment, the nighttime temperature environment, time in bed, respiratory rate and heart rate.

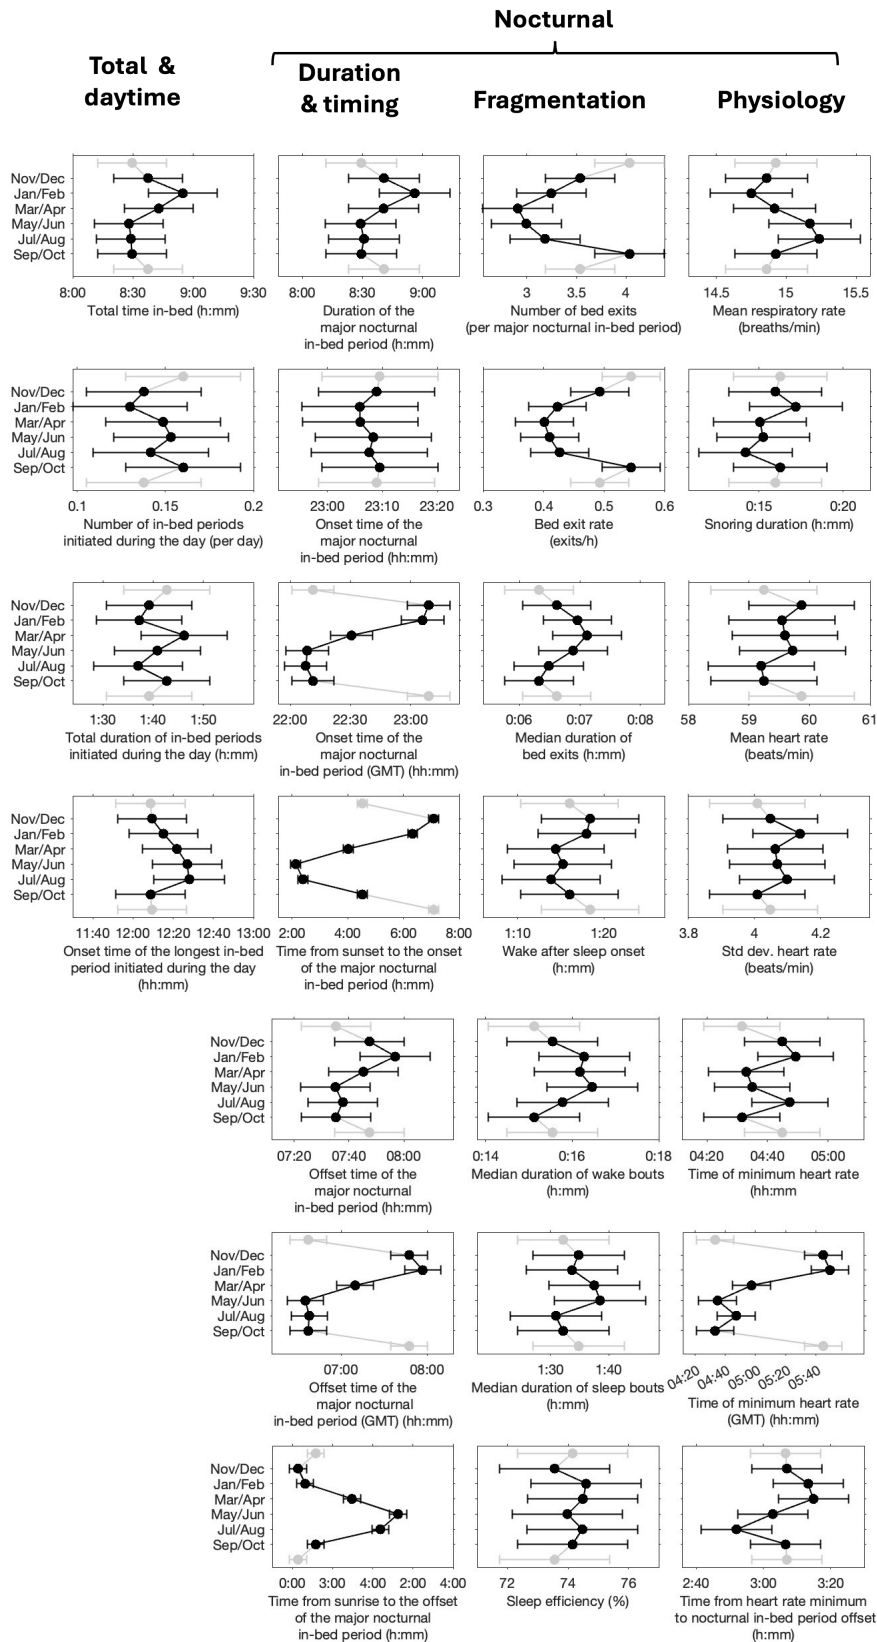


Figure S3: Seasonal variation of in-bed duration, timing and fragmentation, physiology. The data shown are the Least Squares (LS) means from a linear mixed effect model which considers the seasonal variation for each measure controlling for gender, age and diagnosis with participant as a random effect (see Supplementary Table S5). Eight of the 25 measures are also shown in the Fig. 3 of the main text. All measures are included here for ease of visual comparison.



Figure S4: **Individual variation in total time in-bed.** Time courses of the total time in-bed for each participant. Each data point is a single day. The magenta lines show the two-month moving averages.

S4 Tables summarising statistical results

	Two-month period				Hour of the day				Room				Home			
	DF1	DF2	FStat	p	DF1	DF2	FStat	p	DF1	DF2	FStat	p	DF1	DF2	FStat	p
Light (log lux)	5	3153075	83912	<0.0001	23	3153075	186037	<0.0001	3	3153075	14562	<0.0001	69	3153075	3148	<0.0001
Temperature (°C)	5	3144684	227267	<0.0001	23	3144684	7360	<0.0001	3	3144684	2017	<0.0001	69	3144684	38033	<0.0001

Table S2: **Daily and seasonal variation of the light and temperature environment.** Results of a linear fixed effect model for average hourly light (log lux) and temperature (°C) for the fixed effects of hour of the day, two-month period, room and home. Hour, two-month period, room and home were all entered as categorical variables.

	Two-month period			
	DF1	DF2	FStat	p value
Bright light, lounge (hours > 500 lux)	5	26517	1406	<0.0001
Geometric mean daily light, lounge (lux)	5	26517	2034	<0.0001
Mean nocturnal temperature, bedroom (°C)	5	26517	4377	<0.0001
Temperature amplitude, bedroom (°C)	5	26494	764	<0.0001

Table S3: **Seasonal variation of the light and temperature environment.** Results of a linear mixed effect model for various *daily* indoor light and temperature measures with the fixed effect of two-month period and the random effect of home.

	Number of observations	Mean	Standard deviation	Standard error	95th confidence interval (low)	95th confidence interval (high)	Minimum	Maximum	Median	25th percentile	75th percentile	IQR	Intraclass correlation coefficient, ICC
TOTAL TIME IN-BED PER 24 HOURS													
Total time in-bed (h:mm)	70	8:48	2:05	0:15	8:18	9:18	3:11	14:36	8:48	7:45	10:01	2:16	0.52
TIME IN-BED INITIATED DURING THE DAY													
NUMBER & DURATION													
Number of in-bed periods initiated during the day (per day)	70	0.14	0.24	0.03	0.08	0.20	0.00	1.34	0.04	0.01	0.12	0.11	0.33
Total duration of in-bed periods initiated during the day (h:mm)	66	1:39	0:57	0:07	1:24	1:53	0:15	5:19	1:18	0:60	2:09	1:10	0.21
TIMING													
Onset time of the longest in-bed period initiated during the day (hh:mm)	66	12:24	2:13	0:16	11:51	12:56	07:16	16:21	12:40	11:04	14:09	3:06	0.34
TIME IN-BED INITIATED DURING THE NIGHT													
DURATION													
Duration of the major nocturnal in-bed period (h:mm)	70	8:47	2:09	0:15	8:17	9:18	3:11	14:39	8:54	7:36	9:42	2:06	0.51
TIMING													
Onset time of the major nocturnal in-bed period (hh:mm)	70	23:05	1:18	0:09	22:47	23:24	19:07	02:04	23:10	22:17	23:49	1:32	0.41
Onset time of the major nocturnal in-bed period (GMT) (hh:mm)	70	22:31	1:17	0:09	22:13	22:50	18:35	01:30	22:36	21:44	23:13	1:29	0.39
Time from sunset to the onset of the major nocturnal in-bed period (h:mm)	70	4:28	1:19	0:09	4:09	4:47	0:28	7:36	4:25	3:45	5:12	1:27	0.22
Offset time of the major nocturnal in-bed period (hh:mm)	70	07:51	1:33	0:11	07:28	08:13	03:06	11:36	08:05	06:59	08:54	1:56	0.40
Offset time of the major nocturnal in-bed period (GMT) (hh:mm)	70	07:17	1:33	0:11	06:54	07:39	02:23	11:03	07:29	06:25	08:17	1:52	0.38
Time from sunrise to the offset of the major nocturnal in-bed period (h:mm)	70	1:19	1:35	0:11	0:56	1:42	-3:30	5:01	1:31	0:19	2:25	2:07	0.35
FRAGMENTATION													
Number of bed exits (per major nocturnal in-bed period)	70	3.10	2.65	0.32	2.47	3.73	0.11	17.63	2.27	1.52	4.01	2.49	0.32
Bed exit rate (exits/h)	70	0.40	0.37	0.04	0.31	0.48	0.01	1.71	0.27	0.18	0.50	0.32	0.29
Median duration of bed exits (h:mm)	70	0:06	0:04	0:00	0:05	0:07	0:01	0:27	0:05	0:04	0:07	0:03	0.29
Wake after sleep onset (h:mm)	70	1:15	0:41	0:05	1:05	1:25	0:10	3:48	1:10	0:48	1:32	0:45	0.30
Median duration of wake bouts (h:mm)	70	0:15	0:08	0:01	0:13	0:17	0:05	0:39	0:14	0:09	0:19	0:09	0.15
Median duration of sleep bouts (h:mm)	70	1:38	0:57	0:07	1:24	1:51	0:24	4:42	1:21	1:02	2:01	0:59	0.33
Sleep efficiency (%)	70	75.69	13.60	1.63	72.45	78.93	22.83	95.78	77.81	71.52	85.49	13.98	0.51
PHYSIOLOGY													
MEAN & DURATION													
Mean respiratory rate (breaths/min)	70	14.89	2.16	0.26	14.37	15.40	11.42	20.41	14.52	13.31	15.98	2.67	0.85
Snoring duration (h:mm)	70	0:17	0:21	0:02	0:12	0:22	0:00	1:19	0:08	0:03	0:24	0:21	0.41
Mean heart rate (beats/min)	70	59.47	6.69	0.80	57.88	61.07	47.09	75.78	58.93	54.26	64.25	9.99	0.80
Std dev. heart rate (beats/min)	70	3.97	1.07	0.13	3.71	4.22	0.91	6.58	3.80	3.39	4.62	1.22	0.44
TIMING													
Time of minimum heart rate (hh:mm)	70	04:36	1:30	0:11	04:15	04:58	00:36	07:20	04:40	03:38	05:50	2:12	0.24
Time of minimum heart rate (GMT) (hh:mm)	70	04:03	1:31	0:11	03:41	04:24	00:05	06:48	04:04	03:05	05:10	2:05	0.23
Time from heart rate minimum to nocturnal in-bed period offset (h:mm)	70	3:17	1:18	0:09	2:58	3:36	1:21	8:43	3:05	2:23	3:56	1:34	0.21
ENVIRONMENT													
Geometric mean daily light, lounge (lux)	70	46.31	25.14	3.01	40.32	52.31	17.18	155.65	40.12	30.80	58.02	27.22	0.33
Hours bright light, lounge (h:mm > 500 lux)	70	2.60	2.33	0.28	2.04	3.15	0.00	9.56	1.86	0.92	4.02	3.10	0.44
Mean nocturnal temperature, bedroom (°C)	70	21.05	2.20	0.26	20.53	21.57	16.28	25.84	21.00	19.48	22.21	2.73	0.47
Amplitude temperature, bedroom (°C)	70	2.76	1.14	0.14	2.49	3.03	1.07	5.86	2.62	1.91	3.22	1.31	0.40

Table S4: Descriptive statistics for the measures of sleep behaviour and physiology and the light and temperature environment Descriptive statistics describing the distribution of the $n = 70$ participant mean values for the 25 different measures of sleep behaviour and physiology and 4 measures of the light and temperature environment. The intraclass correlation coefficient for each measure is also included. For all measures, the reported mean is the mean of the participant mean values, i.e. from the approximately 26,000 days of data, the individual participant mean values were first calculated. Then the mean of the participant values was found.

	Intercept	Two-month period			Gender				Alzheimer's diagnosis				Initial age			
		DF	Fstat	p	DF	Fstat	p	Man effect	DF	Fstat	p	Not Alzheimer's effect	DF	Fstat	p	Initial age effect (per y)
TOTAL TIME IN-BED PER 24 HOURS																
Total time in-bed (h)	8.41	26138	34.36	4.0E-35	26138	0.11	0.7412	0.18	26138	1.98	0.1593	-0.79	26138	0.03	0.8681	0.005
TIME IN-BED INITIATED DURING THE DAY																
NUMBER & DURATION																
Number of in-bed periods initiated during the day (per day)	0.42	26138	4.69	2.8E-04	26138	0.13	0.7231	0.02	26138	0.21	0.6499	0.03	26138	1.14	0.2849	-0.004
Total duration of in-bed periods initiated during the day (h)	1.13	3276	0.77	5.7E-01	3276	0.00	0.9631	-0.01	3276	0.35	0.5540	-0.15	3276	0.40	0.5270	0.008
TIMING																
Onset time of the longest in-bed period initiated during the day (h)	16.23	3276	1.53	1.8E-01	3276	3.77	0.0522	0.99	3276	0.54	0.4642	-0.39	3276	4.00	0.0455	-0.055
TIME IN-BED INITIATED DURING THE NIGHT																
DURATION																
Duration of the major nocturnal in-bed period (h)	8.30	26138	29.89	2.1E-30	26138	0.01	0.9174	-0.06	26138	2.05	0.1523	-0.82	26138	0.07	0.7940	0.008
TIMING																
Onset time of the major nocturnal in-bed period (h)	0.84	26138	1.17	3.2E-01	26138	0.23	0.6336	0.16	26138	0.36	0.5494	0.21	26138	1.64	0.2002	-0.024
Onset time of the major nocturnal in-bed period (GMT) (h)	-0.14	26138	402.36	0.0E+00	26138	0.24	0.6262	0.16	26138	0.34	0.5614	0.20	26138	1.62	0.2031	-0.023
Time from sunset to the onset of the major nocturnal in-bed period (h)	6.24	26138	6469.65	0.0E+00	26138	0.19	0.6669	0.14	26138	0.33	0.5645	0.20	26138	1.69	0.1933	-0.024
Offset time of the major nocturnal in-bed period (hh:mm)	8.85	26138	24.76	5.7E-25	26138	0.12	0.7334	0.13	26138	2.28	0.1313	-0.63	26138	0.34	0.5592	-0.013
Offset time of the major nocturnal in-bed period (GMT) (h)	7.87	26138	450.52	0.0E+00	26138	0.12	0.7280	0.14	26138	2.32	0.1277	-0.63	26138	0.33	0.5662	-0.013
Time from sunrise to the offset of the major nocturnal in-bed period (h)	1.81	26138	1252.28	0.0E+00	26138	0.14	0.7034	0.15	26138	2.28	0.1311	-0.63	26138	0.32	0.5738	-0.012
FRAGMENTATION																
Number of bed exits (per major nocturnal in-bed period)	6.37	26138	48.87	1.6E-50	26138	5.67	0.0173	-1.55	26138	0.02	0.8843	-0.10	26138	0.27	0.6035	-0.019
Bed exit rate (exits/h)	0.56	26138	40.48	1.3E-41	26138	8.14	0.0043	-0.25	26138	1.01	0.3160	0.09	26138	0.03	0.8626	0.001
Median duration of bed exits (h)	0.04	26138	9.16	1.0E-08	26138	0.04	0.8379	0.00	26138	3.21	0.0733	0.03	26138	0.38	0.5352	0.001
Wake after sleep onset (h)	0.43	26138	3.77	2.1E-03	26138	0.65	0.4204	-0.14	26138	0.00	0.9599	-0.01	26138	1.41	0.2352	0.012
Median duration of wake bouts (h)	0.11	26138	3.35	5.1E-03	26138	0.52	0.4693	0.02	26138	3.24	0.0720	0.06	26138	0.51	0.4747	0.001
Median duration of sleep bouts (h)	0.55	26138	5.86	2.1E-05	26138	0.60	0.4372	0.19	26138	0.04	0.8485	-0.05	26138	0.72	0.3958	0.012
Sleep efficiency (%)	97.81	26138	4.00	1.3E-03	26138	1.09	0.2956	3.54	26138	2.04	0.1530	-5.12	26138	2.30	0.1297	-0.289
NOCTURNAL PHYSIOLOGY																
MEAN & DURATION																
Mean respiratory rate (breaths/min)	11.71	25801	181.86	6.1E-191	25801	0.12	0.7269	0.19	25801	0.62	0.4317	0.46	25801	1.40	0.2363	0.036
Snoring duration (h)	1.03	26138	7.57	4.1E-07	26138	0.65	0.4201	0.07	26138	0.65	0.4191	-0.07	26138	3.94	0.0471	-0.010
Mean heart rate (beats/min)	41.87	25907	25.76	5.0E-26	25907	0.31	0.5801	-0.90	25907	0.03	0.8718	-0.28	25907	6.09	0.0136	0.227
Std dev. heart rate (beats/min)	4.67	25907	5.73	2.7E-05	25907	5.22	0.0223	-0.61	25907	0.42	0.5165	0.18	25907	0.14	0.7082	-0.006
TIMING																
Time of minimum heart rate (h)	6.43	25907	10.28	7.3E-10	25907	0.04	0.8440	-0.08	25907	0.24	0.6242	0.20	25907	1.33	0.2496	-0.025
Time of minimum heart rate (GMT) (h)	5.44	25907	194.39	4.9E-204	25907	0.04	0.8494	-0.07	25907	0.22	0.6356	0.19	25907	1.30	0.2539	-0.025
Time from heart rate minimum to nocturnal in-bed period offset (h)	2.67	25907	12.38	5.1E-12	25907	0.27	0.6027	0.17	25907	5.70	0.0169	-0.81	25907	0.29	0.5917	0.010

Table S5: **Seasonal effects on the duration, timing and fragmentation of bed occupancy and physiology.** Results from a linear mixed effect model for the seasonal variation of the 25 measures of bed occupancy, physiology and a marker of the biological clock controlling for gender, age and diagnosis. One of the participant's did not have a diagnosis, so only 69 of the 70 participants were included in this analysis.

	Intercept	Time-in-study				Hours of bright light (>500 lux)				Mean nocturnal temperature				Temperature amplitude			
		DF	Fstat	p	Time-in-study effect (per year)	DF	Fstat	p	Hours of bright light effect (per h)	DF	Fstat	p	Nocturnal temperature effect (per C°)	DF	Fstat	p	Temperature amplitude effect (per C°)
TOTAL TIME-IN-BED PER 24 HOURS																	
Total time in-bed (h)	8.43	26111	2.07	1.50E-01	0.0428	26111	12.30	4.54E-04	-0.019	26111	0.41	5.23E-01	-0.005	26111	90.80	1.72E-21	0.0925
TIME-IN-BED INITIATED DURING THE DAY																	
NUMBER & DURATION																	
Number of in-bed periods initiated during the day (per day)	0.34	26111	34.62	4.06E-09	0.0295	26111	0.68	4.10E-01	0.001	26111	7.26	7.04E-03	0.003	26111	0.12	7.32E-01	0.0006
Total duration of in-bed periods initiated during the day (h)	1.44	3265	36.23	1.95E-09	0.4125	3265	0.49	4.83E-01	-0.008	3265	1.50	2.21E-01	-0.019	3265	2.97	8.51E-02	0.0408
TIMING																	
Onset time of the longest in-bed period initiated during the day (h)	16.52	3265	5.41	2.01E-02	-0.2696	3265	1.18	2.77E-01	-0.021	3265	0.18	6.67E-01	-0.012	3265	0.38	5.36E-01	0.0249
TIME-IN-BED INITIATED DURING THE NIGHT																	
DURATION																	
Duration of the major nocturnal in-bed period (h)	8.59	26111	10.06	1.52E-03	-0.1004	26111	10.47	1.22E-03	-0.018	26111	3.65	5.62E-02	-0.015	26111	71.41	3.06E-17	0.0873
TIMING																	
Onset time of the major nocturnal in-bed period (h)	1.80	26111	42.23	8.28E-11	-0.1507	26111	3.48	6.22E-02	0.008	26111	64.18	1.18E-15	-0.045	26111	1.60	2.05E-01	-0.0096
Onset time of the major nocturnal in-bed period (GMT) (h)	0.99	26111	55.05	1.21E-13	-0.1736	26111	0.36	5.51E-01	-0.003	26111	86.02	1.91E-20	-0.053	26111	0.04	8.38E-01	0.0016
Time from sunset to the onset of the major nocturnal in-bed period (h)	8.58	26111	44.30	2.87E-11	-0.1639	26111	61.19	5.37E-15	-0.035	26111	339.60	2.35E-75	-0.110	26111	16.21	5.68E-05	0.0323
Offset time of the major nocturnal in-bed period (hh:mm)	10.11	26111	55.96	7.64E-14	-0.2137	26111	2.95	8.58E-02	-0.009	26111	78.44	8.78E-19	-0.061	26111	75.38	4.10E-18	0.0809
Offset time of the major nocturnal in-bed period (GMT) (h)	9.30	26111	67.87	1.83E-16	-0.2366	26111	13.70	2.15E-04	-0.019	26111	97.92	4.78E-23	-0.069	26111	96.53	9.63E-23	0.0920
Time from sunrise to the offset of the major nocturnal in-bed period (h)	2.19	26111	62.85	2.32E-15	-0.2299	26111	10.18	1.42E-03	0.017	26111	7.97	4.77E-03	-0.020	26111	36.27	1.74E-09	0.0570
FRAGMENTATION																	
Number of bed exits (per major nocturnal in-bed period)	7.72	26111	81.46	1.91E-19	-0.5166	26111	13.16	2.87E-04	-0.037	26111	8.98	2.73E-03	-0.042	26111	70.57	4.67E-17	-0.1568
Bed exit rate (exits/h)	0.73	26111	29.99	4.38E-08	-0.0470	26111	4.77	2.89E-02	-0.003	26111	7.33	6.78E-03	-0.006	26111	67.37	2.35E-16	-0.0230
Median duration of bed exits (h)	0.01	26111	0.63	4.28E-01	0.0013	26111	5.23	2.22E-02	-0.001	26111	11.17	8.33E-04	0.001	26111	0.06	8.08E-01	-0.0001
Wake after sleep onset (h)	0.20	26111	8.88	2.88E-03	-0.0469	26111	7.98	4.74E-03	-0.008	26111	13.58	2.29E-04	0.014	26111	1.42	2.34E-01	-0.0061
Median duration of wake bouts (h)	0.01	26111	14.40	1.48E-04	0.0171	26111	0.76	3.85E-01	-0.001	26111	18.67	1.56E-05	0.005	26111	0.74	3.90E-01	0.0013
Median duration of sleep bouts (h)	0.18	26111	199.99	3.09E-45	0.2796	26111	0.99	3.20E-01	0.004	26111	6.18	1.30E-02	0.012	26111	0.49	4.84E-01	-0.0045
Sleep efficiency (%)	100.25	26111	5.75	1.65E-02	-0.4776	26111	0.50	4.78E-01	-0.025	26111	6.04	1.40E-02	-0.119	26111	8.02	4.63E-03	0.1841
NOCTURNAL PHYSIOLOGY																	
MEAN & DURATION																	
Mean respiratory rate (breaths/min)	9.05	25774	23.84	1.05E-06	0.0635	25774	17.89	2.34E-05	-0.010	25774	1753.08	0.00E+00	0.134	25774	4.63	3.14E-02	0.0092
Snoring duration (h)	1.27	26111	142.93	7.40E-33	-0.0733	26111	8.63	3.32E-03	0.003	26111	56.64	5.39E-14	-0.011	26111	0.10	7.55E-01	-0.0006
Mean heart rate (beats/min)	40.39	25880	4.16	4.14E-02	-0.1006	25880	0.12	7.26E-01	0.003	25880	36.33	1.69E-09	0.073	25880	12.90	3.29E-04	0.0581
Std dev. heart rate (beats/min)	4.78	25880	5.95	1.47E-02	-0.0443	25880	5.92	1.50E-02	-0.008	25880	1.05	3.06E-01	-0.005	25880	11.08	8.72E-04	0.0198
TIMING																	
Time of minimum heart rate (h)	7.13	25880	32.25	1.37E-08	-0.2292	25880	0.72	3.95E-01	0.006	25880	12.69	3.68E-04	-0.035	25880	33.73	6.42E-09	0.0766
Time of minimum heart rate (GMT) (h)	6.32	25880	38.83	4.69E-10	-0.2520	25880	0.32	5.71E-01	-0.004	25880	18.63	1.59E-05	-0.043	25880	44.16	3.09E-11	0.0878
Time from heart rate minimum to nocturnal in-bed period offset (h)	3.19	25880	0.24	6.26E-01	-0.0181	25880	6.17	1.30E-02	-0.017	25880	6.62	1.01E-02	-0.023	25880	0.02	8.77E-01	-0.0019

Table S6: Effects of light, temperature and time-in-study on the duration, timing and fragmentation of bed occupancy and on physiology. Linear mixed effect model results for the 25 measures of bed occupancy and physiology, extending the model reported in Table S5 to include environmental variables. Only the results for the additional variables (hours of bright light, mean nocturnal temperature, temperature amplitude and time-in-study) are shown. All other effects are similar to those reported in Supplementary Table S5). One of the participant's did not have a diagnosis, so only 69 of the 70 participants were included in this analysis.

S5 Seasonal desynchrony

The time of the heart rate minimum is a hypothesised marker for the timing of the biological clock with heart rate tending to drop overnight to a minimum and then rising before wake. This can be seen in Fig. 1 and is reproduced in Fig. S5 (a) for the “seasonal” participant. An example for one night is shown in Fig. S5 (b). Around January in the transition from Year 2 to Year 3, the time of the heart rate minimum appears to desynchronise from the 24 h day. Light is the major driver of entrainment to the 24 h day and for the timing of the biological clock. For this participant, the environmental sensors in the home indicate that the indoor light environment is very dim, particularly during the winter months, see Fig. S5 (c), well below recommended light levels [1]. To assess whether the low levels of lighting could be a contributing factor to the observed desynchrony we used a mathematical model which has previously been shown to accurately fit individual mean sleep duration and timing using light collected from wearable sensors [2]. We took the first month of environmental light and bedmat sleep timing data (June of Year 1) and, as in [2], tuned two parameters one for sleep duration and one for sleep timing to create a personalised model. We then took the personalised model and fed in the environmental light to predict sleep timing in all subsequent months in two scenarios. First assuming that there was no feedback from the sleep-wake cycle on to the light-dark cycle. Second assuming that light was gated by sleep. Predicted sleep timing is shown for the two cases in (d). Interestingly, we found that when lights were turned on and off according to when measured bedtime occurred, we found that there was a delay in predicted sleep and circadian timing in the winter months. Whereas, when light is gated by predicted sleep-wake timing, desynchrony in the winter occurs. These two scenarios demonstrate the stabilising effect of imposed lights out / bedtimes on sleep and circadian timing, as highlighted in [3]. One explanation for the difference between the first and second winter is that a period of ill-health leading to changes in routine, combined with the low levels of ambient light could trigger the observed desynchrony.

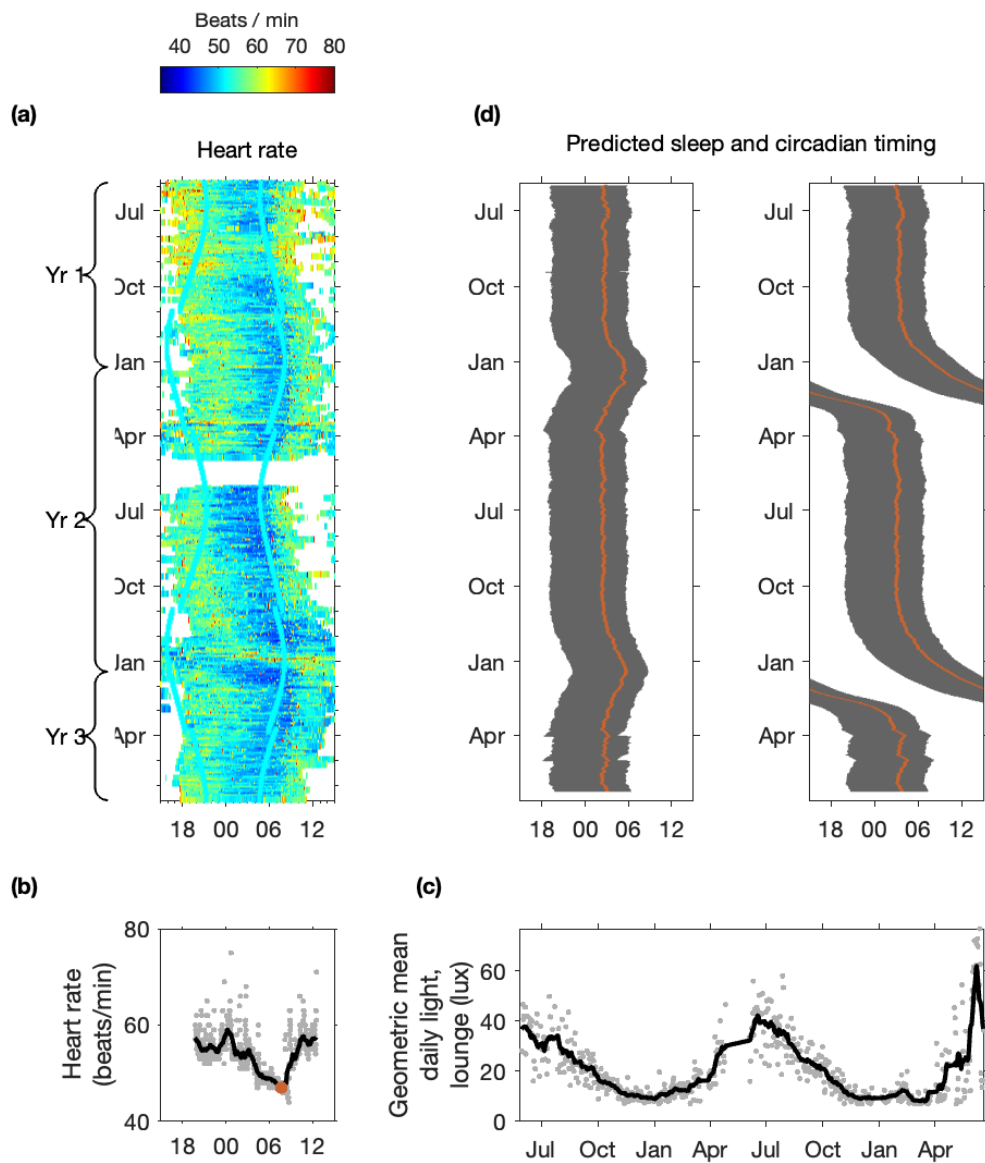


Figure S5: **Desynchrony due to a maladaptive light environment?** a) Raster plot for the heart rate for participant “seasonal”, replicated from Fig. 1 (b). Recording of heart rate during sleep for one night showing how the heart rate dips to a minimum. Superimposed on the raw data is a 60 minute moving average, with the circular marker indicating the minimum. (c) Mean daily light levels in the lounge for participant “seasonal”. (d) Raster plots of sleep predictions. In the left hand panel, it is assumed that light is not gated by sleep. In the right hand panel, it is assumed that the measured light is gated by sleep.

Bibliography

- [1] Brown T. M., Brainard G. C., Cajochen C., Czeisler C. A., Hanifin J. P., Lockley S.W., and et al. Recommendations for daytime, evening, and nighttime indoor light exposure to best support physiology, sleep, and wakefulness in healthy adults. *PLoS Biol.*, 20:e3001571, 2022.
- [2] Skeldon A. C., T. Rodriguez Garcia, S. F. Cleator, C. della Monica, K. K. G. Ravindran, V. L. Revell, and D.-J. Dijk. Method to determine whether sleep phenotypes are driven by endogenous circadian rhythms or environmental light by combining longitudinal data and personalised mathematical models. *PLOS Comput. Biol.*, 19:e1011743, 2023.
- [3] A.C. Skeldon, A.J.K. Phillips, and D.-J. Dijk. The effects of self-selected light-dark cycles and social constraints on human sleep and circadian timing: a modeling approach. *Sci Rep*, 7:45158, 2017.