

## **Supplemental Material**

Humidity and deposition solution play a critical role in virus inactivation by heat treatment on N95 respirators

Nicole Rockey,<sup>a\*</sup> Peter J. Arts,<sup>a\*</sup> Lucinda Li,<sup>a\*</sup> Katherine R. Harrison,<sup>a</sup> Kathryn Langenfeld,<sup>a</sup> William J. Fitzsimmons,<sup>b</sup> Adam S. Lauring,<sup>b</sup> Nancy G. Love,<sup>a</sup> Keith S. Kaye,<sup>b</sup> Lutgarde Raskin,<sup>a</sup> William W. Roberts,<sup>c,d</sup> Bridget Hegarty,<sup>a</sup> Krista R. Wigginton<sup>a#</sup>

<sup>a</sup>Department of Civil & Environmental Engineering, University of Michigan, Ann Arbor, MI, USA

<sup>b</sup>Division of Infectious Diseases, Department of Internal Medicine, University of Michigan Health System, Ann Arbor, MI, USA

<sup>c</sup>Department of Urology, University of Michigan Health System, Ann Arbor, MI, USA

<sup>d</sup>Department of Biomedical Engineering, University of Michigan, Ann Arbor, MI, USA

#Address correspondence to Krista R. Wigginton, kwigg@umich.edu, 734-763-9664

\*Authors contributed equally to this work.

**Control experiment to test the potential impact of drying time.** The MS2 and phi6 virus stock was deposited on coupons and allowed to dry for either one or three hours prior to the heat treatment. The results from this control experiment confirmed that the  $\log_{10}$  inactivation observed through heat treatment was not affected by the drying time of virus droplets on the coupon (Figure S1).

**Virus recovery from N95 respirator coupons.** To assess virus recovery from N95 respirator coupons, 50 uL of each of the virus stocks was suspended into their respective elution solutions. The virus suspensions were extracted and enumerated with the same methods used on the coupons. Recovery rates were calculated as the ratio of the control coupon titer to the virus suspension. Average recovery rates for each virus tested are 56% for IAV, 28% for MHV, 38% for MS2 suspended in PBS, 34% for MS2 suspended in IAV media, 104% for phi6 suspended in PBS, and 7% for phi6 suspended in IAV media.

**Table S1.** Characteristics of SARS-CoV-2 and the viruses used in this study.

Virus	Genome type	Genome size	Particle size (nm)	Enveloped/ Nonenveloped
SARS-CoV-2	(+)ssRNA	29.9 kb	~100	Enveloped
MS2	(+)ssRNA	3.6 kb	~25	Nonenveloped
phi6	dsRNA	13.5 kbp	~85	Enveloped
IAV	(-)ssRNA	13.6 kb	~100	Enveloped
MHV	(+)ssRNA	31.3 kb	~120	Enveloped

**Table S2.** Deposition solutions used in experiments.

Matrix	Description
IAV medium	DMEM supplemented with 0.1875% Fraction V BSA, 25 mM HEPES, and 1% antibiotics (Table S2)
MHV medium	DMEM supplemented with 2% horse serum, L-glutamine, and 1% antibiotics (Table S2)
PBS	1X phosphate buffered saline (Table S3)
PBS + BSA	1X phosphate buffered saline (Invitrogen) supplemented with 0.1875% Fraction V BSA
Saliva	UV sterilized fresh saliva collected from human volunteers

**Table S3.** Composition of phosphate buffer saline solution (Invitrogen, Cat. No. 10010023) used for depositing viruses, as stated by the manufacturer.

Component	Type	Concentration
Potassium Chloride (KCl)	Inorganic Salt	2.7 mM
Potassium Phosphate (NaH <sub>2</sub> PO <sub>4</sub> )	Inorganic Salt	1.8 mM
Sodium Chloride (NaCl)	Inorganic Salt	137 mM
Sodium Phosphate (NaH <sub>2</sub> PO <sub>4</sub> )	Inorganic Salt	10 mM

**Table S4.** Composition of IAV and MHV media used for deposition solutions.

<b>Component</b>	<b>Type</b>	<b>IAV medium</b>	<b>MHV medium</b>
<i>DMEM</i>			
Glycine	Amino Acid	0.4 mM	0.4 mM
L-Arginine hydrochloride	Amino Acid	0.4 mM	0.4 mM
L-Cystine 2HCl	Amino Acid	0.2 mM	0.2 mM
L-Glutamine	Amino Acid	4 mM	2 mM*
L-Histidine hydrochloride-H <sub>2</sub> O	Amino Acid	0.2 mM	0.2 mM
L-Isoleucine	Amino Acid	0.8 mM	0.8 mM
L-Leucine	Amino Acid	0.8 mM	0.8 mM
L-Lysine hydrochloride	Amino Acid	0.8 mM	0.8 mM
L-Methionine	Amino Acid	0.2 mM	0.2 mM
L-Phenylalanine	Amino Acid	0.4 mM	0.4 mM
L-Serine	Amino Acid	0.4 mM	0.4 mM
L-Threonine	Amino Acid	0.8 mM	0.8 mM
L-Tryptophan	Amino Acid	0.08 mM	0.08 mM
L-Tyrosine disodium salt dihydrate	Amino Acid	0.4 mM	0.4 mM
L-Valine	Amino Acid	0.8 mM	0.8 mM
Choline chloride	Vitamin	0.03 mM	0.03 mM
D-Calcium pantothenate	Vitamin	0.01 mM	0.008 mM
Folic acid	Vitamin	0.01 mM	0.009 mM
i-Inositol	Vitamin	0.04 mM	0.04 mM
Niacinamide	Vitamin	0.03 mM	0.03 mM
Pyridoxine hydrochloride	Vitamin	0.02 mM	0.02 mM
Riboflavin	Vitamin	0.001 mM	0.001 mM
Thiamine hydrochloride	Vitamin	0.01 mM	0.01 mM
Calcium Chloride (CaCl <sub>2</sub> ) (anhyd.)	Inorganic Salt	1.8 mM	1.8 mM

Ferric Nitrate ( $\text{Fe}(\text{NO}_3)_3 \cdot 9\text{H}_2\text{O}$ )	Inorganic Salt	0.0002 mM	0.0002 mM
Magnesium Sulfate ( $\text{MgSO}_4$ ) (anhyd.)	Inorganic Salt	0.8 mM	0.8 mM
Potassium Chloride ( $\text{KCl}$ )	Inorganic Salt	5.3 mM	5.4 mM
Sodium Bicarbonate ( $\text{NaHCO}_3$ )	Inorganic Salt	44 mM	44 mM
Sodium Chloride ( $\text{NaCl}$ )	Inorganic Salt	110.3 mM	109.5 mM
Sodium Phosphate monobasic ( $\text{NaH}_2\text{PO}_4 \cdot \text{H}_2\text{O}$ )	Inorganic Salt	0.9 mM	0.9 mM
D-Glucose (Dextrose)	Other	25 mM	25 mM
Phenol red	Other	0.04 mM	0.04 mM
<i>HEPES (N-2-hydroxyethylpiperazine-N-2-ethane sulfonic acid)</i>	Organic chemical	25 mM	-
<i>Bovine serum albumin (Fraction V)</i>	Protein	0.1875%	-
<i>Horse serum</i>	Protein	-	2%
<i>Penicillin/Streptomycin</i>	Antibiotics	1%	1%

\*Not in DMEM, added separately.

**Table S5.** Relative humidity readings from the external instantaneous hygrometer probe for each humidity and temperature controlled oven relative humidity setting. Values were measured in duplicate at 20 minute intervals as the humidity setting was increased and decreased. Average probe measurement is reported with the range of readings in parentheses.

Relative Humidity Setting, %	Temperature Setting, °C	
	72	82
10	0.82 (0.55, 1.08)	0.61 (0.53, 0.68)
20	13.18 (12.72, 13.63)	13.17 (12.48, 13.85)
30	24.48 (24.42, 24.54)	24.76 (24.31, 25.20)
40	36.06 (36.02, 36.10)	35.89 (35.53, 36.25)
50	48.19 (48.12, 48.25)	48.39 (48.33, 48.45)
70	70.42 (70.19, 70.65)	71.12 (70.03, 72.21)
90	88.52 (86.02, 91.02)	90.16 (89.88, 90.43)

**Table S6.** Log<sub>10</sub> inactivation of bacteriophage MS2 across variable heat and humidity treatments and deposition solutions.

Temperature		72°C <sup>a</sup>				82°C <sup>a</sup>			
Deposition solution		PBS	IAV Medium	Saliva	PBS + BSA	PBS	IAV Medium	Saliva	PBS + BSA
Relative humidity (%)	1	0.11 (0.24)	0.36 (0.24)	1.31 (1.44)	1.57	-	-	0.08 (0.19)	0.29 (0.19)
	13	0.41 (0.38)	0.34 (0.38)	5.02 (4.89)	4.75	1.01 (0.99)	0.96	1.53 (1.5)	1.46 (1.5)
	25	1.31 (1.39)	1.46 (1.39)	6.41 (6.35)	6.28	1.41 (1.45)	1.48	2.25 (2.72)	3.18 (2.72)
	36	3.71 (3.72)	3.72 (3.72)	> 6.67 (> 6.71)	> 6.74	-	-	> 6.71 (> 6.37)	6.03 (> 6.37)
	48	> 6.81 <td>6.64 (&gt; 6.38)</td> <td>&gt; 6.57 (&gt; 6.38)</td> <td>&gt; 6.19</td> <td>-</td> <td>-</td> <td>&gt; 6.78 (&gt; 6.55)</td> <td>&gt; 6.32 (&gt; 6.03)</td>	6.64 (> 6.38)	> 6.57 (> 6.38)	> 6.19	-	-	> 6.78 (> 6.55)	> 6.32 (> 6.03)
	71	> 6.85 <td>&gt; 6.62 (&gt; 6.65)</td> <td>&gt; 6.86 (&gt; 6.65)</td> <td>&gt; 6.43</td> <td>-</td> <td>-</td> <td>&gt; 6.58 (&gt; 6.84)</td> <td>&gt; 7.09 (&gt; 6.98)</td>	> 6.62 (> 6.65)	> 6.86 (> 6.65)	> 6.43	-	-	> 6.58 (> 6.84)	> 7.09 (> 6.98)
	89	> 7.11 <td>&gt; 6.62 (&gt; 6.56)</td> <td>&gt; 6.93 (&gt; 6.56)</td> <td>&gt; 6.19</td> <td>-</td> <td>-</td> <td>&gt; 6.83 (&gt; 6.90)</td> <td>&gt; 6.96 (&gt; 7.16)</td>	> 6.62 (> 6.56)	> 6.93 (> 6.56)	> 6.19	-	-	> 6.83 (> 6.90)	> 6.96 (> 7.16)
								2.42 (2.77)	3.12 (0.88)

<sup>a</sup>Replicates shown side-by-side for a given treatment, and arithmetic mean shown in parentheses below replicates. Greater than symbol is used to designate replicates outside of dynamic range. For treatment settings with one or more replicates outside of dynamic range, the arithmetic mean was calculated from the values shown.

**Table S7.** Log<sub>10</sub> inactivation of bacteriophage phi6 across variable heat and humidity treatments and deposition solutions.

Temperature		72°C <sup>a</sup>				82°C <sup>a</sup>				
Deposition solution	PBS	IAV Medium	Saliva	PBS + BSA	PBS	IAV Medium	Saliva	PBS + BSA		
Relative humidity (%)	1	0.85 (0.99)	1.12 (2.58)	2.77 (2.38)	-	-	0.79 (1.48)	2.16 (3.87)	3.08 (1.09)	4.66 (0.76)
	13	1.97 (1.62)	1.27 (4.3)	4.48 (4.12)	1.19 (0.95)	0.70 (1.33)	1.26 (1.40)	3.84 (3.41)	6.61 (6.9)	7.18 (2.62)
	25	3.07 (2.85)	2.63 (> 7.44)	6.02 (> 6.73)	1.78 (1.69)	1.60 (1.34)	1.11 (1.56)	5.60 (5.49)	>8.08 (> 7.63)	>7.18 (> 7.63)
	36	4.88 (5.27)	5.65 (> 7.41)	> 7.70 (> 7.56)	-	-	> 7.25 (> 6.78)	> 6.30 (> 6.89)	> 7.40 (> 6.89)	> 6.38 (> 6.89)
	48	7.14 (7.09)	7.03 (> 7.45)	> 7.76 (> 7.61)	-	-	> 6.97 (> 6.73)	> 6.49 (> 6.73)	> 7.55 (> 6.75)	> 5.95 (> 6.75)
	71	> 6.20 (> 6.63)	> 7.05 (> 7.47)	> 7.83 (> 7.47)	-	-	> 7.08 (> 7.05)	> 7.02 (> 7.47)	> 7.40 (> 7.47)	> 7.54 (> 7.47)
	89	> 6.86 (> 6.79)	> 6.72 (> 6.81)	> 7.62 (> 6.00)	-	-	> 7.07 (> 6.70)	> 6.33 (> 6.70)	> 7.74 (> 7.63)	> 7.51 (> 7.63)

<sup>a</sup>Replicates shown side-by-side for a given treatment, and arithmetic mean shown in parentheses below replicates. Greater than symbol is used to designate replicates outside of dynamic range. For treatment settings with one or more replicates outside of dynamic range, the arithmetic mean was calculated from the values shown.

**Table S8.** Log<sub>10</sub> inactivation of IAV across variable heat and humidity treatments.

Temperature		72°C <sup>a</sup>	82°C <sup>a</sup>
Relative humidity (%)	1	2.56 (2.51)	2.45 (3.30)
	13	3.98 (3.74)	3.50 (> 4.05)
	25	3.61 (> 3.83)	> 4.05 (> 4.19)
	89	> 4.19 (> 4.19)	> 4.19 (> 4.38)

<sup>a</sup>Replicates shown side-by-side for a given treatment, and arithmetic mean shown in parentheses below replicates. Greater than symbol is used to designate replicates outside of dynamic range. For treatment settings with one or more replicates outside of dynamic range, the arithmetic mean was calculated from the values shown.

**Table S9.** Log<sub>10</sub> inactivation of MHV across variable heat and humidity treatments.

Temperature		72°C <sup>a</sup>		82°C <sup>a</sup>	
Relative humidity (%)	1	0.89 (1.25)	1.60	2.89 (2.71)	2.53
	13	2.56 (2.52)	2.48	> 4.17	> 3.45
	25	> (> 3.56)	3.52 3.59	> 3.56	> 3.31
	89	> (> 3.71)	3.83 3.59	> 3.30	> 3.43
					(> 3.37)

<sup>a</sup>Replicates shown side-by-side for a given treatment, and arithmetic mean shown in parentheses below replicates. Greater than symbol is used to designate replicates outside of dynamic range. For treatment settings with one or more replicates outside of dynamic range, the arithmetic mean was calculated from the values shown.

**Table S10.** Results of unpaired t-tests comparing virus log<sub>10</sub>-inactivation values at 72°C and 82°C.

Virus	Treatment		72°C versus 82°C	
	Deposition Solution	RH (%)		
MS2	PBS	<b>1</b>	0.306 (0.79)	
		<b>13</b>	3.87 (0.061)	
		<b>25</b>	34.3 <b>(0.0008)</b>	
	IAV Medium	<b>1</b>	3.56 (0.071)	
	Saliva	<b>13</b>	2.53 (0.13)	
	PBS + BSA	<b>13</b>	10.7 <b>(0.0086)</b>	
	PBS	<b>1</b>	0.702 (0.56)	
phi6		<b>13</b>	3.20 (0.086)	
		<b>25</b>	10.73 <b>(0.0086)</b>	
IAV Medium	<b>1</b>	1.59 (0.25)		
	<b>13</b>	7.79 <b>(0.017)</b>		
Saliva	<b>13</b>	4.41 <b>(0.048)</b>		
PBS + BSA	<b>13</b>	1.37 (0.30)		
IAV	IAV Medium	<b>1</b>	1.44 (0.29)	
MHV	MHV Medium	<b>1</b>	3.68 (0.067)	

<sup>a</sup>Significant p-values are indicated in bold (significance considered p < 0.05).

**Table S11.** Results of unpaired t-tests comparing virus inactivation at different RHs.

Temperature (°C)	Virus	Matrix	t-test (p-value) <sup>a</sup>			
			1% versus 13% RH	13% versus 25% RH	25% versus 36% RH	36% versus 48% RH
72	MS2	PBS	1.08 (0.39)	12.2 <b>(0.0066)</b>	31.0 <b>(0.001)</b>	NA
		IAV Medium	18.38 <b>(0.0029)</b>	9.74 <b>(0.010)</b>	NA	NA
	phi6	PBS	1.69 (0.23)	2.98 (0.10)	5.45 <b>(0.032)</b>	4.68 <b>(0.043)</b>
		IAV Medium	6.50 <b>(0.023)</b>	NA	NA	NA
	IAV	IAV Medium	5.02 <b>(0.038)</b>	NA	NA	NA
	MHV	MHV Medium	3.57 (0.070)	NA	NA	NA
	MS2	PBS	4.32 (0.050)	14.4 <b>(0.0048)</b>	NA	NA
		IAV Medium	5.93 <b>(0.027)</b>	NA	NA	NA
82	phi6	PBS	2.38 (0.14)	4.65 <b>(0.043)</b>	NA	NA
		IAV Medium	3.60 (0.069)	NA	NA	NA

<sup>a</sup>Significant p-values are indicated in bold (significance considered p < 0.05).

NA = Not assessed, because values were below detection limits.

**Table S12.** Results of unpaired t-tests comparing virus  $\log_{10}$  inactivation for viruses in tissue culture media deposition solution.

Treatment		t-test (p-value) <sup>a</sup>					
Temperature (°C)	RH (%)	MS2 versus phi6	MS2 versus IAV	MS2 versus MHV	phi6 versus IAV	phi6 versus MHV	IAV versus MHV
72	1	4.84 <b>(0.040)</b>	7.55 <b>(0.017)</b>	0.52 (0.66)	0.346 (0.76)	3.28 (0.082)	3.51 (0.073)
	13	2.60 (0.12)	4.16 (0.053)	16.8 <b>(0.0035)</b>	1.87 (0.20)	9.65 <b>(0.011)</b>	5.01 <b>(0.038)</b>
82	1	1.27 (0.33)	0.813 (0.50)	0.152 (0.89)	0.592 (0.61)	1.43 (0.29)	1.02 (0.42)

<sup>a</sup>Significant p-values are indicated in bold (significance considered  $p < 0.05$ ).

**Table S13.** Results of unpaired t-tests comparing virus inactivation for an expanded set of deposition solutions.


Temperature (°C)	Virus	RH (%)	t-test (p-value) <sup>a</sup>				
			PBS versus saliva	PBS versus PBS+BSA	PBS versus IAV medium	IAV medium versus saliva	IAV medium versus PBS+BSA
72	MS2	1	NA	NA	6.68 <b>(0.022)</b>	NA	NA
		13	14.2 <b>(0.0049)</b>	22.6 <b>(0.0019)</b>	32.3 <b>(0.0010)</b>	28.4 <b>(0.0012)</b>	24.3 <b>(0.0017)</b>
		25	0.725 (0.54)	2.82 (0.11)	50.0 <b>(0.0004)</b>	66.40 <b>(0.0002)</b>	7.73 <b>(0.016)</b>
	phi6	1	NA	NA	6.70 <b>(0.022)</b>	NA	NA
		13	1.58 (0.25)	0.81 (0.50)	6.81 <b>(0.021)</b>	11.0 <b>(0.0081)</b>	15.4 <b>(0.0042)</b>
		25	4.88 <b>(0.040)</b>	4.81 <b>(0.041)</b>	NA	NA	NA
82	MS2	1	3.85 (0.061)	3.50 (0.073)	7.07 <b>(0.019)</b>	5.00 <b>(0.038)</b>	5.36 <b>(0.033)</b>
		13	1.61 (0.25)	8.55 <b>(0.013)</b>	NA	NA	NA
	phi6	1	0.569 (0.63)	0.955 (0.44)	2.29 (0.15)	3.52 (0.072)	3.66 (0.067)
		13	1.50 (0.27)	2.25 (0.15)	6.71 <b>(0.021)</b>	10.5 <b>(0.0089)</b>	9.02 <b>(0.012)</b>

<sup>a</sup>Significant p-values are indicated in bold (significance considered p < 0.05).


**Table S14.** Results of unpaired t-tests comparing  $\log_{10}$  inactivation of MS2 and phi6 for an expanded set of deposition solutions and treatment settings.

Treatment			t-test (p-value) <sup>a</sup>
Temperature (°C)	Deposition Solution	RH (%)	MS2 versus phi6
72	PBS	1	4.08 (0.055)
		13	3.54 (0.071)
		25	6.30 <b>(0.024)</b>
		36	4.03 (0.057)
	IAV Medium	1	4.84 <b>(0.040)</b>
		13	2.60 (0.12)
	Saliva	13	0.162 (0.89)
		25	2.54 (0.13)
82	PBS + BSA	13	2.1 (0.17)
		25	2.7 (0.12)
	PBS	1	4.68 <b>(0.043)</b>
		13	1.14 (0.37)
		25	5.43 <b>(0.032)</b>
	IAV Medium	1	1.27 (0.33)
	Saliva	1	1.43 (0.29)
		13	2.14 (0.17)
	PBS + BSA	1	0.0440 (0.97)
		13	2.98 (0.10)


<sup>a</sup>Significant p-values are indicated in bold (significance considered p < 0.05).

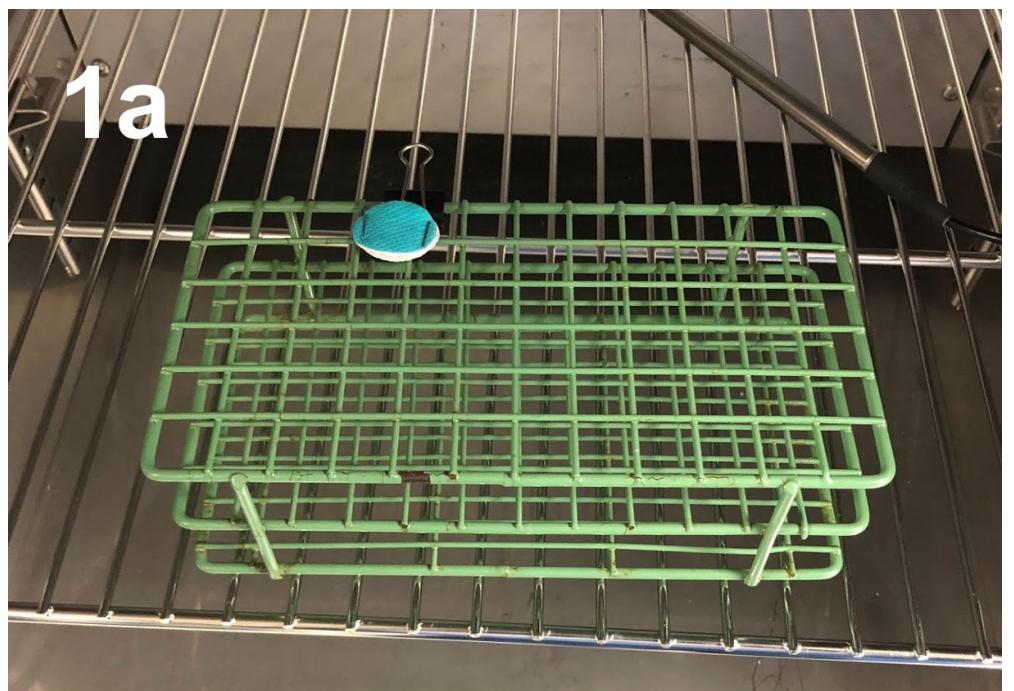

**Figure S1.** Experimental setup of 2a) a N95 respirator coupon attached to a coated metal rack with metal binder clip and 2b) the rack with a coupon placed in the temperature and humidity-controlled oven.

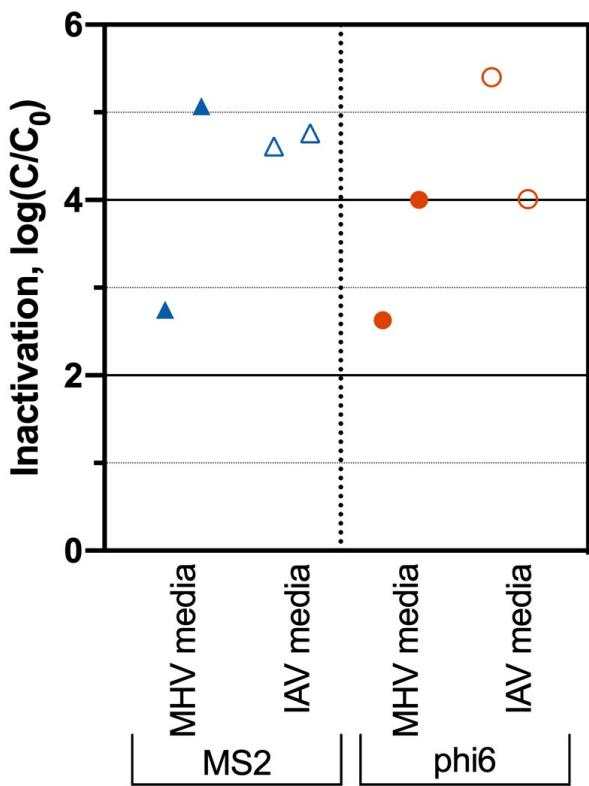

**Figure S2.** Inactivation of bacteriophages at 82°C and 13% in MHV media and IAV media. Independent experimental replicates ( $N = 2$ ) are shown for each virus at each condition.

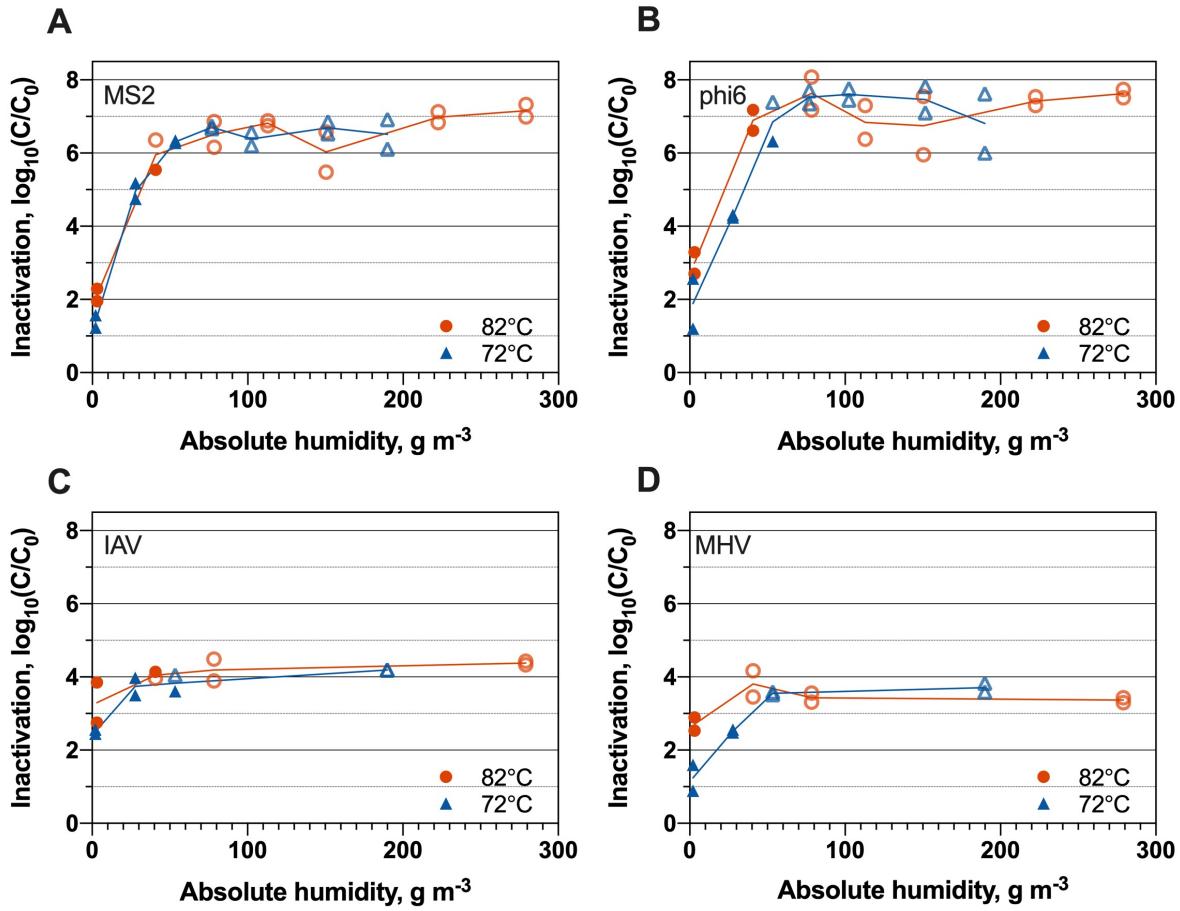

**Figure S3.** Virus inactivation as a function of absolute humidity for a) MS2 bacteriophage, b) phi6 bacteriophage, c) IAV, and d) MHV. Open faded symbols indicate virus inactivation beyond assay detection limits. Independent experimental replicates ( $N = 2$ ) are shown for each virus at each condition.