


Supplementary Figure 1. (A) Demographics of patient population with a positive antibody signal following a negative original PCR result (n=9) out of 68 patients with a negative original PCR result. (B) Detection of antibodies against SARS-CoV-2 by the EuroImmun IgG ELISA (S protein) and the GSD IgG ELISA (N protein) in patients with an original negative PCR result for the virus causing COVID-19.

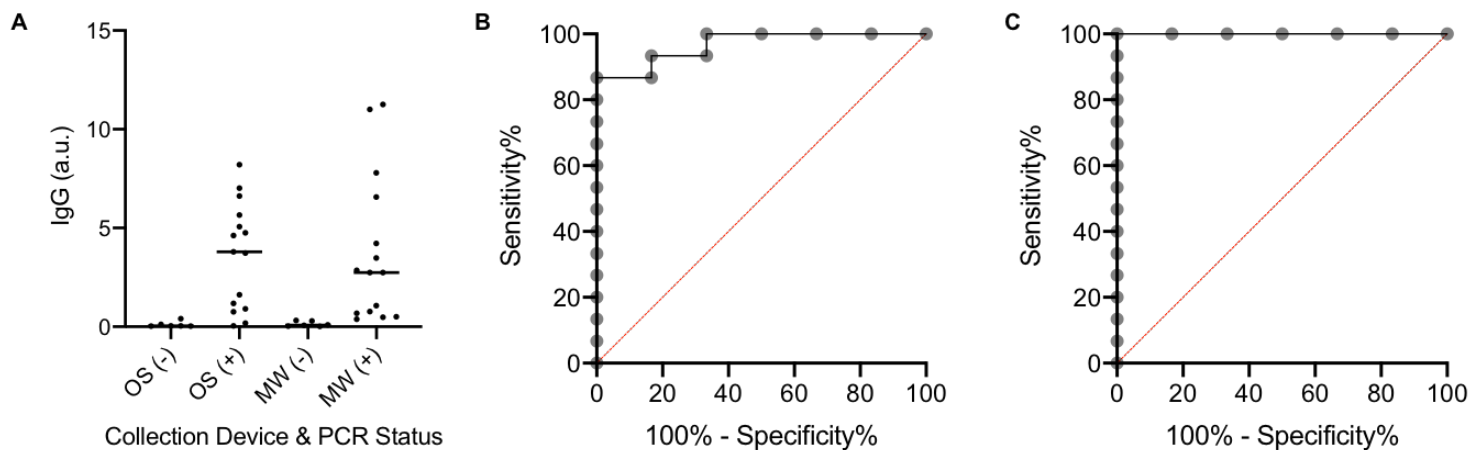

Supplementary Figure 2. (A) An in-house formulated mouthwash (MW) and a saliva-based antibody collection device from OraSure Technologies (OS) were compared for antibody detection in 6 PCR-negative and 15 PCR-positive samples. (B) Samples collected from this cohort of participants using the OraSure antibody collection device gave 87% sensitivity and 100% specificity (AUC = 0.967) with a cutoff value of 0.58. (C) Samples collected from this cohort of participants using the in-house formulated mouthwash provided 100% sensitivity and 100% specificity (AUC = 1.000) with a cutoff value of 0.35.

	Female only	Male only	Data >21d out from symptom onset	Data >41 days out from symptom onset	Data >61 days out from symptom onset
Sensitivity	75.6	89.2	84.9	90.5	71.4
Specificity	97.4	96.4	95.6	95.6	95.6
AUC	0.943	0.981	0.975	0.983	0.943

Supplementary Table 1. Data were stratified to test whether focusing on certain subpopulations within our clinical cohort improved test sensitivity and specificity