

Evaluating aerosol and splatter during orthodontic debonding: implications for the COVID-19 pandemic

Hayley Llandro^{1,2}, James R Allison^{1,2}, Charlotte C Currie^{1,2}, David C Edwards^{1,2}, Charlotte Bowes^{1,2}, Justin Durham^{1,2}, Nicholas Jakubovics², Nadia Rostami², Richard Holliday^{1,2}

Affiliations

1. Newcastle Upon Tyne Hospitals NHS Foundation Trust, Newcastle Upon Tyne, United Kingdom
2. School of Dental Sciences, Newcastle University, United Kingdom

Corresponding Author: Richard Holliday; School of Dental Sciences, Newcastle University, Newcastle upon Tyne, NE1 7RU; richard.holliday@newcastle.ac.uk


Supplementary Material

		Rig contamination. Distance from centre (m)									
Min		0	0.5	1	1.5	2	2.5	3	3.5	4	Total
Mean (SD)											
Max		11.16	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00
Sum		91.5	1.88	0.01	0.00	0.00	0.00	0.00	0.00	0.00	1.64
[n]		(127.8)	(5.78)	(0.05)	(0.00)	(0.00)	(0.00)	(0.00)	(0.00)	(0.00)	(17.3)
Surface area (mm ²)		238.88	26.24	0.25	0.00	0.00	0.00	0.00	0.00	0.01	238.88
		274.61	45.31	0.36	0.00	0.00	0.00	0.00	0.00	0.01	320.29
		[3]	[24]	[24]	[24]	[24]	[24]	[24]	[24]	[24]	[195]
		0	0	0	0	0	0	0.00	0	0	0
		2328	1019	251	31 (153)	0 (0)	9 (45)	59 (290)	0 (0)	31 (151)	208
Fluorescence (RFU)		(2917)	(3335)	(1230)	749	0	220	1421	0	738	(1334)
		5601	13207	6028	749	0	220	1421	0	738	13207
		6984	24451	6028	[24]	[24]	[24]	[24]	[24]	[24]	40591
		[3]	[24]	[24]							[195]
Operator contamination											
		Left body	Right Body	Left arm	Right arm	Left leg	Right leg	Head	Visor[#]	Mask[§]	Total
Surface area (mm ²)		37.41	0.00	0.09	0.00	0.00	0.00	0.00	0.00	0.00	0.00
		23.62	0.00	12.76	0.00	0.01	0.00	0.00	4.26	0.00	3.87
		(16.9)	(0.00)	(11.2)	(0.00)	(0.02)	(0.00)	(0.01)	(7.00)	(0.01)	(8.54)
		37.41	0.02	21.5	0.00	0.04	0.00	0.01	27.49	0.02	37.41
		70.86	0.02	38.3	0.00	0.04	0.00	0.01	76.71	0.04	185.94
	[3]	[3]	[3]	[3]	[3]	[3]	[3]	[18]	[9]	[48]	
Fluorescence (RFU)		0	0	0	0	0	0	0	0	0	0
		8473	1271	776	359	0 (0)	0 (0)	0 (0)	1205	21 (63)	1136
		(8598)	(2202)	(1345)	(622)	0	0	0	(1931)	190	(2961)
		17189	3814	2329	1077	0	0	0	5847	190	17189
		25420	3814	2329	1077	[3]	[3]	[3]	21691	[9]	54521
	[3]	[3]	[3]	[3]				[18]		[48]	
Assistant contamination											
		Left body	Right Body	Left arm	Right arm	Left leg	Right leg	Head	Visor[#]	Mask[§]	Total
Surface area (mm ²)		0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00
		0.00	0.00	0.10	2.17	0.00	0.42	0.00	0.00	0.00	0.14
		(0.00)	(0.00)	(0.17)	(2.55)	(0.00)	(0.07)	(0.00)	(0.00)	(0.00)	(0.75)
		0.00	0.00	0.29	4.97	0.00	0.13	0.00	0.00	0.00	4.98
		0.00	0.00	0.29	6.51	0.00	0.13	0.00	0.00	0.00	6.93
	[3]	[3]	[3]	[3]	[3]	[3]	[3]	[3]	[18]	[9]	[48]
Fluorescence (RFU)		0	0	0	0	0	0	0	0	0	0
		0 (0)	0 (0)	0 (0)	645	0 (0)	0 (0)	0 (0)	27 (113)	0 (0)	50 (255)
		0	0	0	(921)	0	0	0	481	0	1700
		0	0	0	1700	0	0	0	481	0	2417
		[3]	[3]	[3]	1936	[3]	[3]	[3]	[18]	[9]	[48]
				[3]							
Mannequin contamination											
		Upper left		Upper right		Lower left		Lower right		Total	
Surface area (mm ²)			12.34		1.58		0.03		0.00	0.00	
			13.59 (1.24)		4.46 (2.97)		2.79 (4.58)		0.01 (0.01)	5.21	
			14.82		7.51		8.03		0.02	(5.82)	
			40.78		13.37		8.36		0.03	14.82	
			[3]		[3]		[3]		[3]	62.55	
										[12]	
Fluorescence (RFU)			0		666		0		0	0	
			4303 (5911)		1931 (1326)		124 (175)		0 (0)	1723	
			11044		3312		248		0	(3280)	
			12910		5795		248		0	11044	
			[3]		[3]		[2]		[3]	18953	
										[11]	

Supplementary Table 1. Positive control (high-speed air turbine crown preparation with assistant held dental suction). Dental aerosol and splatter as measured by contaminated surface area using image analysis or by spectrofluorometric analysis. The data from an average of three repetitions for all samples at each location are included together.

All visor samples combined

§ All mask samples combined

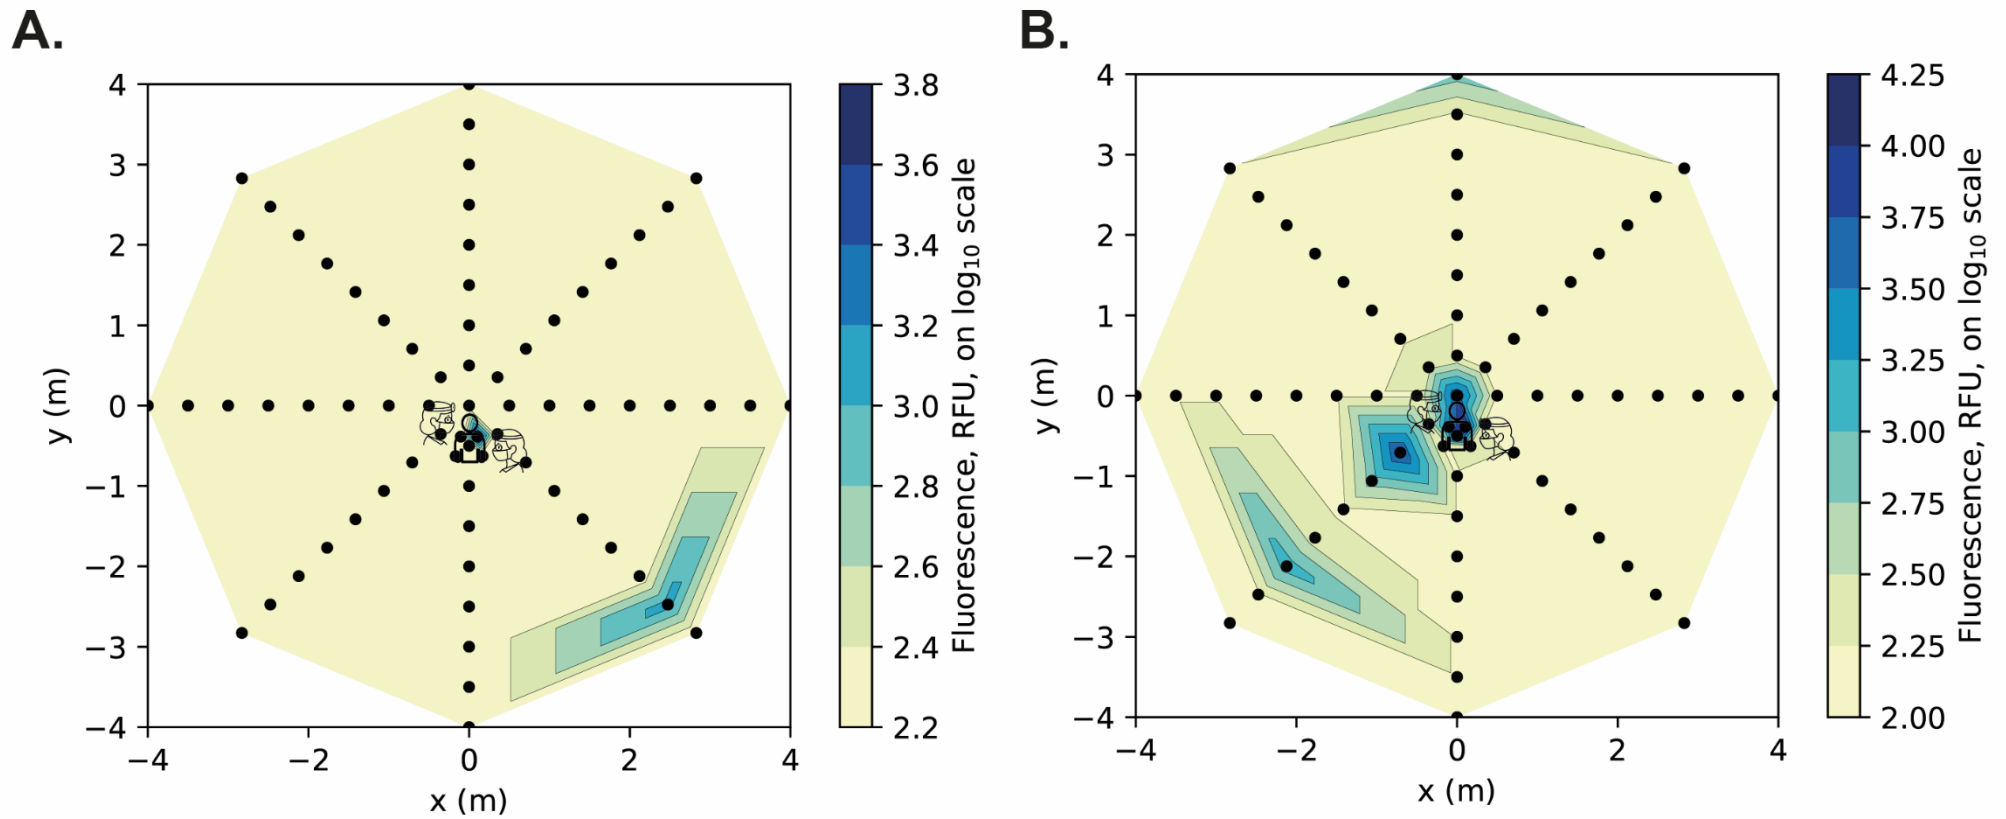

Supplementary Figure 1. Heatmaps presenting spectrofluorometric analysis data. A, Orthodontic debonding procedure. B, positive control (anterior crown preparation). For each coordinate, the maximum value recorded from three repetitions of each clinical procedure was used. Logarithmic transformation was performed on the data (Log₁₀). Note the scale includes the full dimensions of the experimental rig. RFU: relative fluorescence units.