


Supplemental Figure 4

A

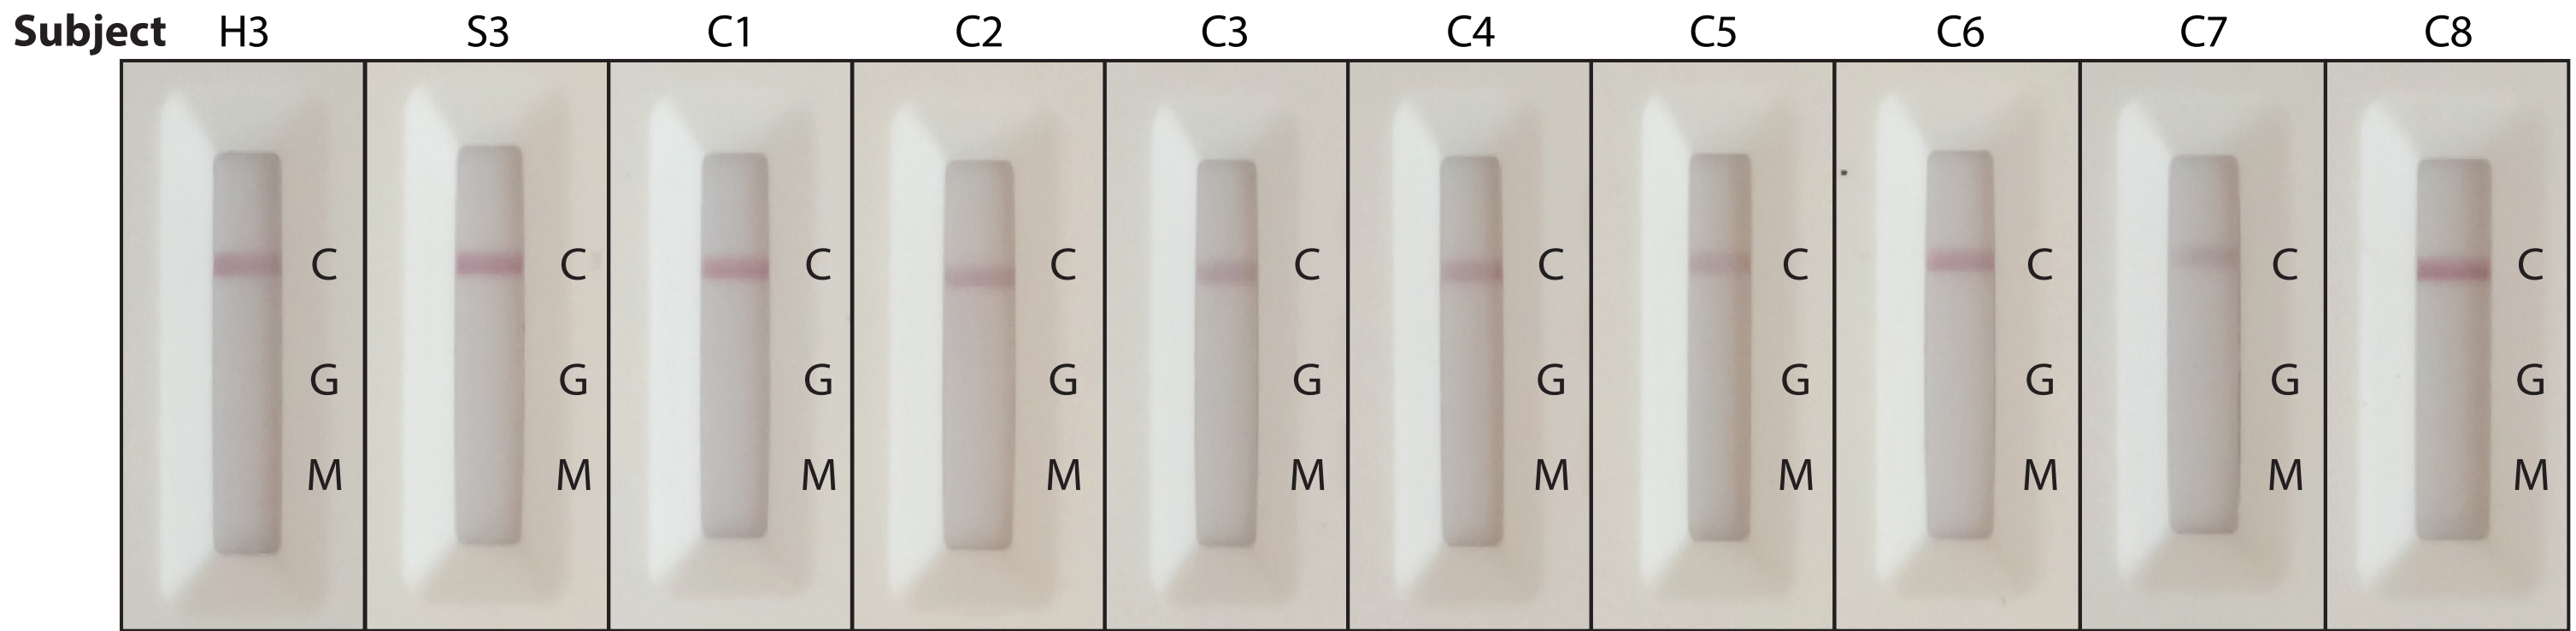

B

Operator ID: CD
System serial number: 40676

Results List Report
Released

C / P	Module	SID	Name	Assay	Result	Flags	Code	Date / Time
LAS	1	26	C-08	COV-2 IgG	0.01 Index Negative			06.25.2020 11:18
LAS	1	49	C-07	COV-2 IgG	0.03 Index Negative			06.25.2020 11:17
LAS	1	47	C-06	COV-2 IgG	0.02 Index Negative			06.25.2020 11:17
LAS	1	21	C-05	COV-2 IgG	0.02 Index Negative			06.25.2020 11:16
LAS	1	20	C-04	COV-2 IgG	0.03 Index Negative			06.25.2020 11:15
LAS	1	19	C-03	COV-2 IgG	0.24 Index Negative			06.25.2020 11:15
LAS	1	18	C-02	COV-2 IgG	0.01 Index Negative			06.25.2020 11:15
LAS	1	17	C-01	COV-2 IgG	0.01 Index Negative			06.25.2020 11:14
LAS	1	16	B-04	COV-2 IgG	6.07 Index Positive			06.25.2020 11:14
LAS	1	15	B-03	COV-2 IgG	6.23 Index Positive			06.25.2020 11:14
LAS	1	11	B-02	COV-2 IgG	2.66 Index Positive			06.25.2020 11:13
LAS	1	10	B-01	COV-2 IgG	4.07 Index Positive			06.25.2020 11:13